



**Model 675**  
**High Performance Arbitrary Waveform Generator**  
**AFG Mode Programming Manual**  
(Active Technology AWG-4010 Series)  
Rev 1.4, Dec 2020



## TABLE OF CONTENTS

<b>1. PREFACE</b> .....	<b>9</b>
1.1 ABBREVIATIONS AND TERMS.....	9
1.2 REVISION HISTORY .....	9
<b>2. SYNTAX AND COMMANDS</b> .....	<b>13</b>
2.1 COMMAND SYNTAX.....	13
2.1.1 Syntax Overview.....	13
2.1.2 Command and Query Structure .....	13
2.1.3 Command Entry .....	15
2.1.4 Parameter Types .....	16
2.1.5 SCPI Commands and Queries .....	18
3.1 THE REGISTERS.....	19
3.1.1 The Standard Event Status Register (SESR).....	19
3.1.2 The Status Byte Register (SBR) .....	20
3.1.3 The Operation Condition Register (OCR) .....	20
3.1.4 The Operation Event Register (OEVR) .....	21
3.1.5 The Questionable Event Register (QEV), Questionable Condition Register (QCR) and Questionable Enable Register (QENR).....	22
3.1.6 DESER, ESER, SRER Registers .....	22
<b>4. REMOTE CONTROL</b> .....	<b>23</b>
4.1 PREREQUISITE .....	23
4.1.1.1 <i>AT INSTRUMENT COMMUNICATOR</i> .....	28
4.2 COMMAND GROUPS.....	30
Date and Time Commands .....	30
4.2.1 File System Commands.....	30
4.2.2 Memory Commands.....	31
4.2.3 Mass Memory Commands .....	31
4.2.4 Output Commands.....	32
4.2.5 Display Commands.....	32
4.2.6 Source Commands .....	33
4.2.7 Device commands .....	43
4.2.8 Status Commands.....	44
4.2.9 Synchronization Group Commands.....	44

4.2.10 System Group Commands .....	45
4.2.11 Trace Commands .....	45
4.2.12 Trigger Group Commands .....	46
4.3 COMMAND DESCRIPTIONS .....	47
<b>5. COMMAND ERRORS .....</b>	<b>154</b>
<b>6. PROGRAMMING EXAMPLES.....</b>	<b>156</b>
6.1 EXAMPLE SCRIPT.....	156
6.2 PYTHON EXAMPLES.....	156
6.3 MATLAB EXAMPLES .....	157
6.4 LABVIEW EXAMPLES .....	157
6.5 MICROSOFT C# EXAMPLE.....	163
6.6 MICROSOFT C++ EXAMPLE .....	165

## LIST OF TABLES

Table 1: Abbreviations and terms .....	9
Table 2: Revision History.....	12
Table 3: Syntax symbols and their meanings .....	13
Table 4: Message symbols and their meanings.....	14
Table 5: Message terminator and meaning .....	15
Table 6: Parameter types, their descriptions, and examples .....	16
Table 7: String symbol and meaning .....	16
Table 8: SI prefixes and their indexes .....	17
Table 9: Standard Event Status Register (SESR) .....	20
Table 10: Status Byte Register (SBR).....	20
Table 11: Operation Condition Register (OCR) .....	21
Table 12: Models and available parameters.....	30
Table 13: Date and Time Commands .....	30
Table 14: File System Commands.....	31
Table 15: Memory Commands.....	31
Table 16: Mass Memory Commands .....	32
Table 17: Output Commands.....	32
Table 18: HCopy Command .....	32
Table 19: Source Commands .....	43
Table 20: Device Commands.....	43
Table 21: Status Commands.....	44
Table 22: Synchronization group commands .....	45
Table 23: System group commands .....	45
Table 24: Trace group commands.....	46
Table 25: Trigger group commands.....	47
Table 26: DATE.....	48
Table 27: TIME.....	48
Table 28: FILEsystem:CATalog.....	48
Table 29: FILEsystem:COPY.....	49
Table 30: FILEsystem:CWDirectory .....	49
Table 31: FILEsystem:DElete .....	50
Table 32: FILEsystem:HARDdisk.....	50
Table 33: FILEsystem:LOCK .....	51
Table 34: FILEsystem:MDIRectory.....	51
Table 35: FILEsystem:UDISK? .....	51
Table 36: MEMory:RECall.....	52

Table 37: MEMory:SAVE.....	52
Table 38: MEMory:STATe:DELeTe .....	53
Table 39: MEMory:STATe:LOCK .....	53
Table 40: MEMory:STATe:VALId? .....	54
Table 41: *RCL .....	54
Table 42: *SAV .....	54
Table 43: HCOPy:SDUMp[:IMMediate] .....	55
Table 44: DISPlay:CHANnel .....	55
Table 45: MMEMory:LOAD:STATe.....	56
Table 46: MMEMory:STORe:STATe.....	56
Table 47: OUTPut[n][:STATe] .....	57
Table 48: OUTPut[n]:IMPedance .....	57
Table 49: OUTPut[n]:LOW:IMPedance .....	58
Table 50: OUTPut[n]:POLarity .....	58
Table 51: [SOURce[n]]:AM[:DEPTTh] .....	59
Table 52: [SOURce[n]]:AM:INTernal:FREQuency .....	59
Table 53: [SOURce[n]]:AM:INTernal:FUNcTion.....	60
Table 54: [SOURce[n]]:AM:INTernal:FUNcTion:EFILe .....	61
Table 55: [SOURce[n]]:AM:SOURce .....	61
Table 56: [SOURce[n]]:AM:STATe.....	61
Table 57: [SOURce[n]]:BURSt:MODE.....	62
Table 58: [SOURce[n]]:BURSt:NCYCles.....	63
Table 59: [SOURce[n]]:BURSt[:STATe] .....	63
Table 60: [SOURce[n]]:BURSt:TDELay.....	64
Table 61: [SOURce[n]]:COMBine:FEED .....	64
Table 62: [SOURce[n]]:FM[:DEViation] .....	65
Table 63: [SOURce[n]]:FM:INTernal:FREQuency.....	65
Table 64: [SOURce[n]]:FM:INTernal:FUNcTion.....	66
Table 65: [SOURce[n]]:FM:INTernal:FUNcTion:EFILe .....	66
Table 66: [SOURce[n]]:FM:SOURce .....	67
Table 67: [SOURce[n]]:FM:STATe .....	67
Table 68: [SOURce[n]]:FREQuency[:CW   :FIXed] .....	68
Table 69: [SOURce[n]]:FREQuency:MODE .....	69
Table 70: [SOURce[1   2]]:FREQuency:STARt .....	69
Table 71: [SOURce[n]]:FREQuency:STOP .....	70
Table 72: [SOURce[n]]:FSKey[:FREQuency] .....	70
Table 73: [SOURce[n]]:FSKey:INTernal:RATE .....	71
Table 74: [SOURce[n]]:FSKey:SOURce .....	71
Table 75: [SOURce[n]]:FSKey:STATe.....	72

Table 76: [SOURCE[n]]:PSKey[:FREQUENCY] .....	72
Table 77: [SOURCE[n]]:PSKey:PHASe[:ADJUST] .....	73
Table 78: [SOURCE[n]]:PSKey:SOURCe .....	73
Table 79: [SOURCE[n]]:PSKey:STATe .....	74
Table 80: [SOURCE[n]]:FUNCTioN:EFILe .....	74
Table 81: [SOURCE[n]]:FUNCTioN:RAMP:SYMMetry .....	75
Table 82: [SOURCE[n]]:FUNCTioN[:SHAPE] .....	76
Table 83: [SOURCE[n]]:INITDELay .....	77
Table 84: [SOURCE[n]]:PHASe[:ADJUST] .....	78
Table 85: [SOURCE[n]]:PM[:DEViation] .....	78
Table 86: [SOURCE[n]]:PM:INTernal:FREQUENCY .....	79
Table 87: [SOURCE[n]]:PM:INTernal:FUNCTioN .....	79
Table 88: [SOURCE[n]]:PM:INTernal:FUNCTioN:EFILe .....	80
Table 89: [SOURCE[n]]:PM:SOURCe .....	80
Table 90: [SOURCE[n]]:PM:STATe .....	81
Table 91: [SOURCE[n]]:POWER[:LEVel][:IMMediate][:AMPLitude] .....	81
Table 92: [SOURCE[n]]:PULSe:DCYCLe .....	82
Table 93: [SOURCE[n]]:PULSe:TRANSition[:LEADing] .....	83
Table 94: [SOURCE[n]]:PULSe:TRANSition:TRAILing .....	83
Table 95: [SOURCE[n]]:PULSe:WIDTh .....	84
Table 96: [SOURCE[n]]:PWM:INTernal:FREQUENCY .....	84
Table 97: [SOURCE[n]]:PWM:INTernal:FUNCTioN .....	85
Table 98: [SOURCE[n]]:PWM:INTernal:FUNCTioN:EFILe .....	86
Table 99: [SOURCE[n]]:PWM:SOURCe .....	86
Table 100: [SOURCE[n]]:PWM:STATe .....	87
Table 101: [SOURCE[n]]:PWM[:DEViation]:DCYCLe .....	87
Table 102: [SOURCE]:ROSCillator:FREQUENCY .....	88
Table 103: [SOURCE]:ROSCillator:SOURCe .....	88
Table 104: [SOURCE[n]]:SWEep:NSTEP .....	89
Table 105: [SOURCE[n]]:SWEep:HTIME .....	89
Table 106: [SOURCE[n]]:SWEep:MODE .....	90
Table 107: [SOURCE[n]]:SWEep:RTIME .....	90
Table 108: [SOURCE[n]]:SWEep:SPACing .....	91
Table 109: [SOURCE[n]]:SWEep:SPACing:EFILe .....	92
Table 110: [SOURCE[n]]:SWEep:TIME .....	92
Table 111: [SOURCE[n]]:VOLTage[:LEVel][:IMMediate]:HIGH .....	93
Table 112: [SOURCE[n]]:VOLTage[:LEVel][:IMMediate]:LOW .....	93
Table 113: [SOURCE[n]]:VOLTage[:LEVel][:IMMediate]:OFFSet .....	94
Table 114: [SOURCE[n]]:VOLTage[:LEVel][:IMMediate][:AMPLitude] .....	94

Table 115: [SOURce[n]]:VOLTage:UNIT .....	95
Table 116: [SOURce[n]]:VOLTage:VOCM.....	96
Table 117: [SOURce[n]]:PULSe:TRANSition[:LEADing] .....	97
Table 118: [SOURce[n]]:PULSe:TRANSition:TRAIling.....	98
Table 119:[SOURce[n]]:DOUBLEPULSe:PULSe[m]:WIDTh.....	98
Table 120:[SOURce[n]]:DOUBLEPULSe:PULSe[m]:WIDTh.....	99
Table 121: [SOURce[n]]:COUPLE:STATe .....	100
Table 122: [SOURce[n]]:COUPLE:AMPLitude:STATe .....	101
Table 123: [SOURce[n]]:COUPLE:AMPLitude:RATio .....	102
Table 124: [SOURce[n]]:COUPLE:AMPLitude:OFFSet .....	102
Table 125: [SOURce[n]]:COUPLE:OFFSet:STATe.....	103
Table 126: [SOURce[n]]:COUPLE:OFFSet:RATio .....	104
Table 127: [SOURce[n]]:COUPLE:OFFSet:OFFSet .....	105
Table 128: [SOURce[n]]:COUPLE:FREQuency:STATe.....	106
Table 129: [SOURce[n]]:COUPLE:FREQuency:RATio .....	106
Table 130: [SOURce[n]]:COUPLE:FREQuency:OFFSet.....	107
Table 131: [SOURce[n]]:COUPLE:PHASe:STATe .....	108
Table 132: [SOURce[n]]:COUPLE:PHASe:RATio.....	109
Table 133: [SOURce[n]]:COUPLE:PHASe:OFFSet .....	110
Table 134: [SOURce[n]]:COUPLE:DCYCLe:STATe.....	111
Table 135: [SOURce[n]]:COUPLE:DCYCLe:RATio .....	111
Table 136: [SOURce[n]]:COUPLE:DCYCLe:OFFSet.....	112
Table 137: [SOURce[n]]:COUPLE:LEADing:STATe .....	113
Table 138: [SOURce[n]]:COUPLE:LEADing:RATio.....	114
Table 139: [SOURce[n]]:COUPLE:LEADing:OFFSet .....	115
Table 140: [SOURce[n]]:COUPLE:TRAIling:STATe .....	116
Table 141: [SOURce[n]]:COUPLE:LEADing:RATio.....	117
Table 142: [SOURce[n]]:COUPLE:TRAIling:OFFSet .....	118
Table 143: [SOURce[n]]:COUPLE:SYMMetry:STATe.....	118
Table 144: [SOURce[n]]:COUPLE:SYMMetry:RATio .....	119
Table 145: [SOURce[n]]:COUPLE:SYMMetry:OFFSet .....	120
Table 146: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:AMPLitude:STATe .....	121
Table 147: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:AMPLitude:RATio .....	122
Table 148: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:AMPLitude:OFFSet .....	123
Table 149: Command [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:STATe .....	124
Table 150: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:RATio.....	125
Table 151: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:OFFSet .....	126
Table 152: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:STATe .....	127
Table 153: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:RATio.....	128

Table 154: [SOURce[n]]:COUPLE:LEADing:OFFSet .....	129
Table 155: [SOURce[n]]:COUPLE:DOUBLePULSe:PULSe[m]:WIDTh:STATe .....	129
Table 156: [SOURce[n]]:COUPLE:DOUBLePULSe:PULSe[m]:WIDTh:RATio .....	130
Table 157: [SOURce[n]]:COUPLE:DOUBLePULSe:PULSe[m]:WIDTh:OFFSet .....	131
Table 158: [SOURce[n]]:COUPLE:DOUBLePULSe:PULSe[m]:DELay:STATe .....	132
Table 159: [SOURce[n]]:COUPLE:DOUBLePULSe:PULSe[m]:DELay:RATio .....	133
Table 160: [SOURce[n]]:COUPLE:DOUBLePULSe:PULSe[m]:DELay:OFFSet .....	134
Table 161: [SOURce[n]]:VOLTage:LIMit:HIGH .....	135
Table 162: [SOURce[n]]:VOLTage:LIMit:LOW .....	135
Table 163: AFGControl:START.....	136
Table 164: AFGControl:STOP.....	136
Table 165: AFGControl:STATus .....	136
Table 166: AFGControl:COpy .....	137
Table 167: AFGControl:AWGSwitch .....	137
Table 168: *RST .....	137
Table 169: SYSTem:BEEPer[:IMMediate] .....	138
Table 170: SYSTem:BEEPer:STATe .....	138
Table 171: SYSTem:ERRor[:NEXT] .....	139
Table 172: SYSTem:KCLick[:STATe] .....	139
Table 173: SYSTem:TLOCK[:STATe] .....	140
Table 174: SYSTem:ULANguage? .....	140
Table 175: SYSTem:VERsion? .....	140
Table 176: TRACe[n][:DATA] .....	141
Table 177: TRACe[n]:POINts? .....	142
Table 178: TRACe[n]:RECall .....	142
Table 179: TRACe[n]:SAVE .....	143
Table 180: STATus:OPERation[:EVENT]? .....	143
Table 181: STATus:OPERation:CONDition? .....	144
Table 182: STATus:OPERation:ENABle .....	144
Table 183: STATus:QUESTionable[:EVENT]? .....	144
Table 184: STATus:QUESTionable:CONDition? .....	145
Table 185: STATus:QUESTionable:ENABle .....	145
Table 186: STATus:PRESet .....	145
Table 187: *CLS.....	146
Table 188: *ESE .....	146
Table 189: *ESR? .....	147
Table 190: *SRE .....	147
Table 191: *STB? .....	148
Table 192: *OPC .....	148



Table 193: *WAI .....	149
Table 194: *TRG .....	149
Table 195: TRIGger[:SEQuence][:IMMediate] .....	149
Table 196: ABORT .....	150
Table 197: TRIGger[:SEQuence]:SOURce .....	150
Table 198: TRIGger[:SEQuence]:SLOPe .....	150
Table 199: TRIGger[:SEQuence]:THREshold .....	151
Table 200: TRIGger[:SEQuence]:TIMer .....	151
Table 201: TRIGger[m]:OUTPut:AMPLitude .....	152
Table 202: TRIGger[m]:OUTPut:DELay .....	153
Table 203: TRIGger[m]:OUTPut:STATe .....	153
Table 204 TRIGger[m]:OUTPut:LINK .....	154

# 1. PREFACE

Scope of this document is to describe the use of SCPI commands with the Model 675 High Performance Arbitrary Waveform Generator when used in Function Generator Operational Mode (AFG).

## 1.1 ABBREVIATIONS AND TERMS

Abbreviation	Description
SW	Software
UI	User Interface
API	Application Programming Interface
SCPI	Standard Commands for Programmable Instruments
AFG	Arbitrary Function Generator
VISA	Virtual Instrument Software Architecture

**Table 1: Abbreviations and terms**

## 1.2 Revision History

Rev.	Document Changes	Date
1.3	[SOURce[n]]:FUNCtion[:SHAPE] - Added Double Pulse carrier Added: [SOURce[n]]:DOUBLEPULSe:PULSe[m]:AMPLitude [SOURce[n]]:DOUBLEPULSe:PULSe[m]:TRANSition[:LEADing] [SOURce[n]]:DOUBLEPULSe:PULSe[m]:TRANSition:TRAILing [SOURce[n]]:DOUBLEPULSe:PULSe[m]:WIDTh [SOURce[n]]:DOUBLEPULSe:PULSe[m]:DELay	

1.4	<p>Added:</p> <p>[SOURce[n]]:COUPLE:STATe  [SOURce[n]]:COUPLE:AMPLitude:STATe  [SOURce[n]]:COUPLE:AMPLitude:RATio  [SOURce[n]]:COUPLE:AMPLitude:OFFSet  [SOURce[n]]:COUPLE:OFFSet:STATe  [SOURce[n]]:COUPLE:OFFSet:RATio  [SOURce[n]]:COUPLE:OFFSet:OFFSet  [SOURce[n]]:COUPLE:FREQuency:STATe  [SOURce[n]]:COUPLE:FREQuency:RATio  [SOURce[n]]:COUPLE:FREQuency:OFFSet  [SOURce[n]]:COUPLE:PHASe:STATe  [SOURce[n]]:COUPLE:PHASe:RATio  [SOURce[n]]:COUPLE:PHASe:OFFSet  [SOURce[n]]:COUPLE:DCYClE:STATe  [SOURce[n]]:COUPLE:DCYClE:RATio  [SOURce[n]]:COUPLE:DCYClE:OFFSet  [SOURce[n]]:COUPLE:LEADing:STATe  [SOURce[n]]:COUPLE:LEADing:RATio  [SOURce[n]]:COUPLE:LEADing:OFFSet  [SOURce[n]]:COUPLE:TRAIling:STATe  [SOURce[n]]:COUPLE:TRAIling:RATio  [SOURce[n]]:COUPLE:TRAIling:OFFSet  [SOURce[n]]:COUPLE:SYMMetry:STATe  [SOURce[n]]:COUPLE:SYMMetry:RATio  [SOURce[n]]:COUPLE:SYMMetry:OFFSet</p> <p>[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:AMPLitude:STATe  [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:AMPLitude:RATio  [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:AMPLitude:OFFSet</p> <p>[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:STATe  [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:RATio  [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:OFFSet</p> <p>[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:STATe  [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:RATio  [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:OFFSet</p>	19 September 2019
-----	--	-------------------------

	<p>[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:WIDTH:STATE  [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:WIDTH:RATIo  [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:WIDTH:OFFSet</p> <p>[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:DELay:STATE  [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:DELay:RATIo  [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:DELay:OFFSet</p> <p>[SOURce[n]]:VOLTage:LIMit:HIGH  [SOURce[n]]:VOLTage:LIMit:LOW</p>	
--	--	--

**Table 2: Revision History**

## 2. SYNTAX AND COMMANDS

### 2.1 COMMAND SYNTAX

#### 2.1.1 Syntax Overview

Control the operations and functions of the instrument through the LAN interface using commands and queries. The related topics listed below describe the syntax of these commands and queries. The topics also describe the conventions that the instrument uses to process them. See the Command Groups topic for a listing of the commands by command group or use the index to locate a specific command.

Refer to the following table for the symbols that are used.

Symbol	Meaning
< >	Defined element
::=	Is defined as
	Exclusive OR
{ }	Group; one element is required
[ ]	Optional; can be omitted
...	Previous elements can be repeated
( )	Comment

**Table 3: Syntax symbols and their meanings**

#### 2.1.2 Command and Query Structure

##### Overview

Commands consist of set commands and query commands (usually called commands and queries). Commands modify instrument settings or tell the instrument to perform a specific action. Queries cause the instrument to return data and status information.

Most commands have both a set form and a query form. The query form of the command differs from the set form by its question mark on the end.

For example, the set command *OUTPut1:STATe ON* has a query form *OUTPut1:STATe?*.

Not all commands have both a set and a query form. Some commands have only set and some have only query.

##### Messages

A command message is a command or query name followed by any information the instrument needs to execute the command or query. Command messages may contain five element types, defined in the following table.

Symbol	Meaning
<Header>	This is the basic command name. If the header ends with a question mark, the command is a query. The header may begin with a colon (:) character. If the command is concatenated with other commands, the beginning colon is required. Never use the beginning colon with command headers beginning with a star (*).
<Mnemonic>	This is a header subfunction. Some command headers have only one mnemonic. If a command header has multiple mnemonics, a colon (:) character always separates them from each other.
<Argument>	This is a quantity, quality, restriction, or limit associated with the header. Some commands have no arguments while others have multiple arguments. A <space> separates arguments from the header. A <comma> separates arguments from each other.
<Comma>	A single comma is used between arguments of multiple-argument commands. Optionally, there may be white space characters before and after the comma.
<Space>	A white space character is used between a command header and the related argument. Optionally, a white space may consist of multiple white space characters.

**Table 4: Message symbols and their meanings**

## Commands

Commands cause the instrument to perform a specific function or change one of the settings. Commands have the structure:

[:]<Header>[<Space><Argument>[<Comma><Argument>]...]

A command header consists of one or more mnemonics arranged in a hierarchical or tree structure. The first mnemonic is the base or root of the tree and each subsequent mnemonic is a level or branch of the previous one. Commands at a higher level in the tree may affect those at a lower level. The leading colon (:) always returns you to the base of the command tree.

## Queries

Queries cause the instrument to return status or setting information.

Queries have the structure:

[:]<Header>?

[:]<Header>?[<Space><Argument>[<Comma><Argument>]...]

### 2.1.3 Command Entry

#### Rules

The following rules apply when entering commands:

- You can enter commands in upper or lower case.
- You can precede any command with white space characters. White space characters include any combination of the ASCII control characters 00 through 09 and 0B through 20 hexadecimal (0 through 9 and 11 through 32 decimal).
- The instrument ignores commands consisting of any combination of white space characters and line feeds.

#### Abbreviating

You can abbreviate many instrument commands. Each command in this documentation shows the abbreviations in capitals. For example, enter the command *SOURce1:VOLTage* simply as *SOUR:VOLT*.

#### Concatenating

Use a semicolon (;) to concatenate any combination of set commands and queries. The instrument executes concatenated commands in the order received. When concatenating commands and queries, follow these rules:

1. Separate completely different headers by a semicolon and by the beginning colon on all commands except the first one.  
For example, the commands *SOURce1:VOLTage 1V* and *SOURce1:VOLTage:OFFSet 0.5V*, can be concatenated into the following single command:  
*SOURce1:VOLTage 1V;; SOURce1:VOLTage:OFFSet 0.5V*
2. Never precede a star (\*) command with a semicolon (;) or colon (:).

#### Terminating

This documentation uses <EOM> (end of message) to represent a message terminator.

Symbol	Meaning
<EOM>	Message terminator

**Table 5: Message terminator and meaning**

For messages sent to the instrument, the end-of-message terminator must be the END message (EOI asserted concurrently with the last data byte). The instrument always terminates messages with LF and EOI. It allows white space before the terminator. For example, it allows CR LF.



## 2.1.4 Parameter Types

Parameters are indicated by angle brackets, such as <file\_name>. There are several different types of parameters, as listed in the following table. The parameter type is listed after the parameter. Some parameter types are defined specifically for the instrument command set and some are defined by SCPI.

Parameter type	Description	Example
Boolean	Boolean numbers or values	ON or 1 OFF or 0
NR1 numeric	Integers	0, 1, 15, -1
NR2 numeric	Decimal numbers	1.2, 3.141, -6.5
NR3 numeric	Floating point numbers	3.1415E+9
NRf numeric	Flexible decimal numbers that may be type NR1, NR2, or NR3	See NR1, NR2, and NR3 examples in this table
String	Alphanumeric characters (must be within quotation marks)	"Testing 1, 2, 3"

**Table 6: Parameter types, their descriptions, and examples**

### Quoted String

Some commands accept or return data in the form of a quoted string, which is simply a group of ASCII characters enclosed by a single quote (') or double quote ("). For example: "this is a quoted string". This documentation represents these arguments as follows:

Symbol	Meaning
<QString >	Quoted string of ASCII text

**Table 7: String symbol and meaning**

A quoted string can include any character defined in the 7-bit ASCII character set. Follow these rules when you use quoted strings:

1. Use the same type of quote character to open and close the string. For example: "this is a valid string".
2. You can mix quotation marks within a string as long as you follow the previous rule. For example, "this is an 'acceptable' string".
3. You can include a quote character within a string simply by repeating the quote. For example: "here is a "" mark".
4. Strings can have upper or lower case characters.
5. A carriage return or line feed embedded in a quoted string does not terminate the string, but is treated as just another character in the string.

Here are some invalid strings:

- "Invalid string argument" (quotes are not of the same type)
- "test<EOI>" (termination character is embedded in the string)

### Units and SI Prefix

If the decimal numeric argument refers to voltage, frequency, impedance, or time, express it using SI units instead of using the scaled explicit point input value format <NR3>. (SI units are units that conform to the System International d'Unites standard.) For example, use the input format 200 mV or 1.0 MHz instead of 200.0E-3 or 1.0E+6, respectively, to specify voltage or frequency.

Omit the unit when you describe commands, but include the SI unit prefix. Enter both uppercase and lowercase characters. The following list shows examples of units you can use with the commands.

- V for voltage (V).
- HZ for frequency (Hz).

The SI prefixes, which must be included, are shown in the following table. You can enter both uppercase and lowercase characters.

SI prefix <sup>1</sup>	Corresponding power
EX	10 <sup>18</sup>
PE	10 <sup>15</sup>
T	10 <sup>12</sup>
G	10 <sup>9</sup>
MA	10 <sup>6</sup>
K	10 <sup>3</sup>
M	10 <sup>-3</sup>
U <sup>2</sup>	10 <sup>-6</sup>
N	10 <sup>-9</sup>
P	10 <sup>-12</sup>
F	10 <sup>-15</sup>
A	10 <sup>-18</sup>

**Table 8: SI prefixes and their indexes**

1. Note that the prefix m/M indicates 10<sup>-3</sup> when the decimal numeric argument denotes voltage or time, but indicates 10<sup>6</sup> when it denotes frequency.
2. Note that the prefix u/U is used instead of "µ".

Since M (m) can be interpreted as 1E-3 or 1E6 depending on the units, use mV for V, and MHz for Hz.


The SI prefixes need units.

Correct: 10MHz, 10E+6Hz, 10E+6  
Incorrect: 10M

### 2.1.5 SCPI Commands and Queries

The Arbitrary Function Generator uses a command language based on the SCPI standard. The SCPI (Standard Commands for Programmable Instruments) standard was created by a consortium to provide guidelines for remote programming of instruments. These guidelines provide a consistent programming environment for instrument control and data transfer. This environment uses defined programming messages, instrument responses and data formats that operate across all SCPI instruments, regardless of manufacturer.

The SCPI language is based on a hierarchical or tree structure that represents a subsystem (see following figure). The top level of the tree is the root node; it is followed by one or more lower-level nodes.

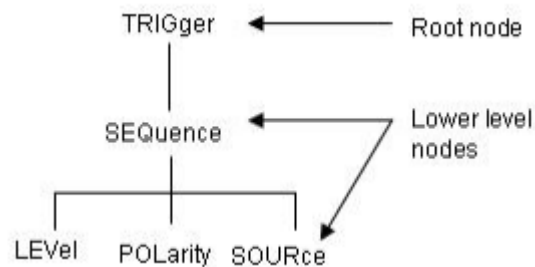

You can create commands and queries from these subsystem hierarchy trees. Commands specify actions for the instrument to perform. Queries return measurement data and information about parameter settings.

### 3.1 The Registers

#### 3.1.1 The Standard Event Status Register (SESR)

BIT	Name	Description
7 (MSB)	PON Power On.	Shows that the instrument was powered on. On completion, the diagnostic tests also set this bit.
6	URQ User Request.	Indicates that an application event has occurred. *See preceding note.
5	CME Command Error.	Shows that an error occurred while the instrument was parsing a command or query.
4	EXE Execution Error	Shows that an error executing a command or query
3	DDE Device Error	Shows that a device error occurred
2	QYE Query Error	Either an attempt was made to read the Output Queue when no data was present or pending, or that data in the Output Queue was lost
1	RQC Request Control	This is not used
0(LSB)	OPC Operation Complete	Shows that the operation is complete. This bit is set when all pending operations

BIT	Name	Description
		complete following an *OPC command

Table 9: Standard Event Status Register (SESR)

### 3.1.2 The Status Byte Register (SBR)

BIT	Name	Description
7 (MSB)	-	Not used
6	RQS Request Service	Obtained from a serial poll. Shows that the instrument requests service from the GPIB controller.
6	MSS Master Status Summary	Obtained from *STB? query. Summarizes the ESB and MAV bits in the SBR.
5	ESB Event Status Bit	Shows that status is enabled and present in the SESR.
4	MAV Message Available	Shows that output is available in the Output Queue
3	-	Not used
2	-	Not used
1	-	Not used
0 (LSB)	-	Not used

Table 10: Status Byte Register (SBR)

### 3.1.3 The Operation Condition Register (OCR)

BIT	Name	Description
7 (MSB)	WTRIG CH8	Waiting for trigger. Indicates whether the instrument is waiting for trigger on CH8.
6	WTRIG CH7	Waiting for trigger. Indicates whether the instrument is waiting for trigger on CH7.
5	WTRIG CH6	Waiting for trigger. Indicates whether the instrument is waiting for trigger on CH6.
4	WTRIG CH5	Waiting for trigger. Indicates whether the instrument is waiting for trigger on CH5.
3	WTRIG CH4	Waiting for trigger. Indicates whether the instrument is waiting for trigger on CH4.
2	WTRIG CH3	Waiting for trigger. Indicates whether the instrument is waiting for trigger on CH3.
1	WTRIG CH2	Waiting for trigger. Indicates whether the instrument is waiting for trigger on CH2.
0 (LSB)	WTRIG CH1	Waiting for trigger. Indicates whether the instrument is waiting for trigger on CH1.

**Table 11: Operation Condition Register (OCR)**

### 3.1.4 The Operation Event Register (OEVR)

This register has the same content as the OCR register.

3.1.5 The Questionable Event Register (QEVR), Questionable Condition Register (QCR) and Questionable Enable Register (QENR).

All these registers are not used.

3.1.6 DESER, ESER, SRER Registers

DESER, ESER, and SRER allow you to select which events are reported to the Status Registers and the Event Queue.

Each Enable Register acts as a filter to a Status Register (the DESER also acts as a filter to the Event Queue) and can prevent information from being recorded in the register or queue. Each bit in an Enable Register corresponds to a bit in the Status Register it controls. In order for an event to be reported to a bit in the Status Register, the corresponding bit in the Enable Register must be set to one. If the bit in the Enable Register is set to zero, the event is not recorded.

Various commands set the bits in the Enable Registers. The Enable Registers and the commands used to set them are described as follows.

The Device Event Status Enable Register (DESER). This register controls which types of events are reported to the SESR and the Event Queue. The bits in the DESER correspond to those in the SESR. Use the DESE command to enable and disable the bits in the DESER. Use the DESE? query to read the DESER.

Event Status Enable Register (ESER).  
This 8-bit register mask the SESR register, it controls which types of events are summarized by the Event Status Bit (ESB) in the SBR.  
Use the \*ESE command to set the bits in the ESER. Use the \*ESE? query to read it.

Service Request Enable Register (SRER).  
This register controls which bits in the SBR generate a Service Request and are summarized by the Master Status Summary (MSS) bit.  
Use the \*SRE command to set the SRER. Use the \*SRE? query to read the register.  
The RQS bit remains set to one until either the Status Byte Register is read with a Serial Poll or the MSS bit changes back to a zero.

## 4. REMOTE CONTROL

You can connect your instrument to a network for printing, file sharing, and Internet access, among other functions. Consult with your network administrator and use the standard Windows utilities to configure the instrument for your network.

The instrument can be controlled using VXI-11 (LAN) protocol. It allows you to control the instrument remotely by using SCPI commands.

### 4.1 Prerequisite


#### NI-VISA

VISA provides the programming interface between the hardware and development environments such as Visual Studio .NET, LabVIEW, LabWindows/CVI, Measurement Studio for Microsoft Visual Studio and MatLab. NI-VISA is the National Instruments implementation of the VISA I/O standard. NI-VISA includes software libraries, interactive utilities such as NI I/O Trace and the VISA Interactive Control, and configuration programs through Measurement & Automation Explorer for all your development needs.

1. Connect your LAN cable to the instrument.
2. On the Client-PC you must install the latest NIVISA package that you can find here <http://search.ni.com/nisearch/app/main/p/bot/no/ap/tech/lang/it/pg/1/sn/cat-nav:du,n8:3.1637,ssnav:sup/>




### 3. Launch the NI-MAX tool on the Client-PC

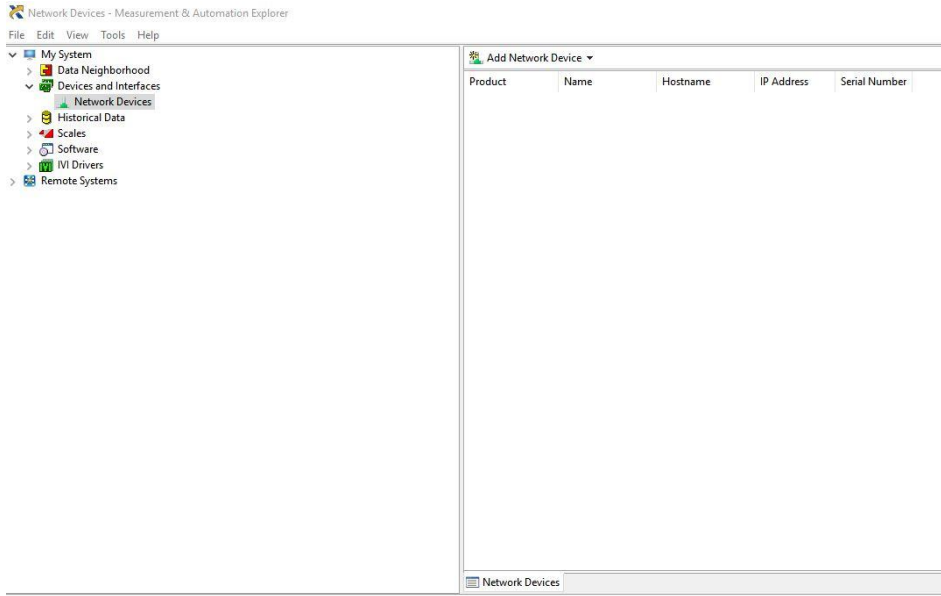


Press Add Network Device → VISA TCP/IP Resource...


### 4. Select Auto-detect of LAN Instrument

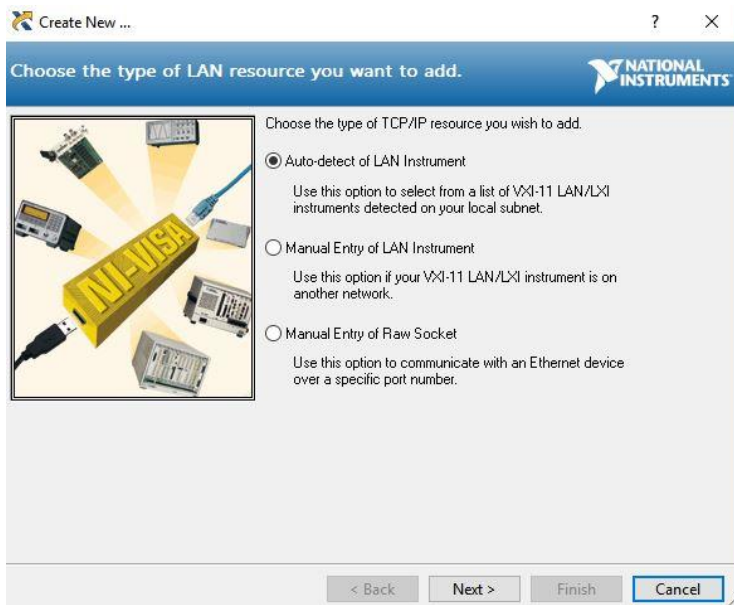


5. The panel will retrieve the discovered instruments on the LAN network, you should select the AT-FUNCTION series one.

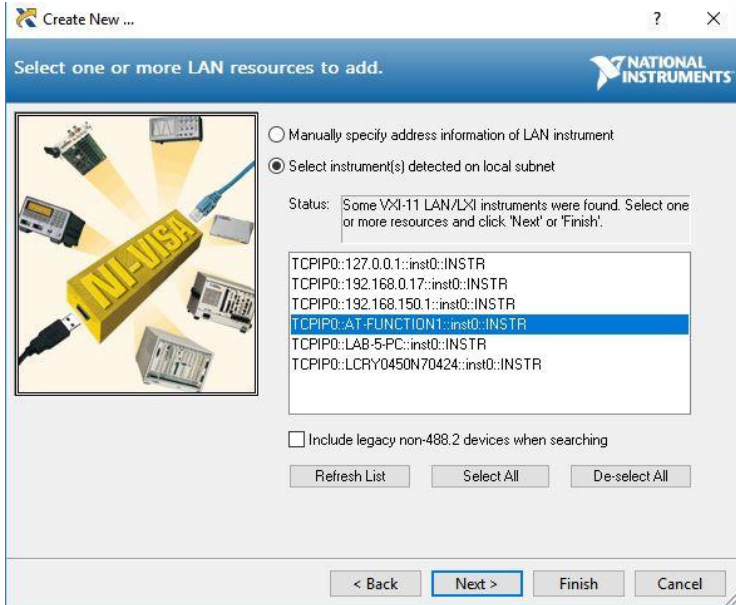


6. Specify an Alias for the selected resource

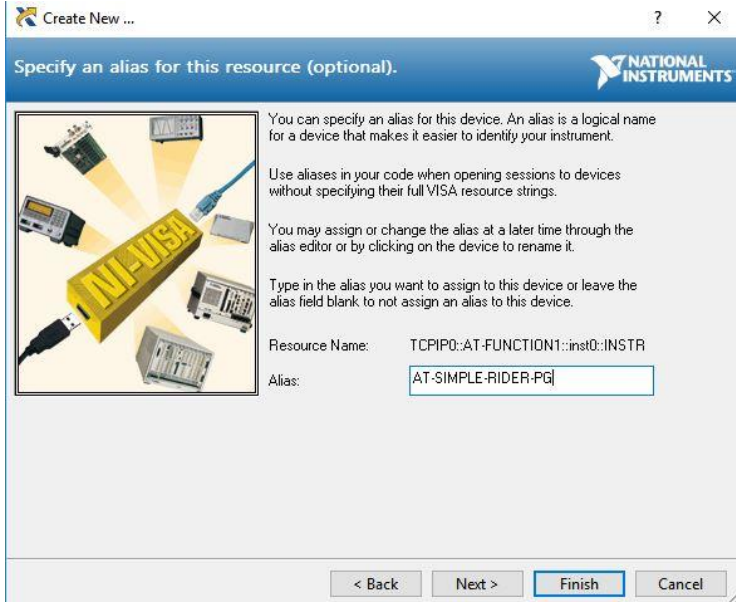


7. Press Finish

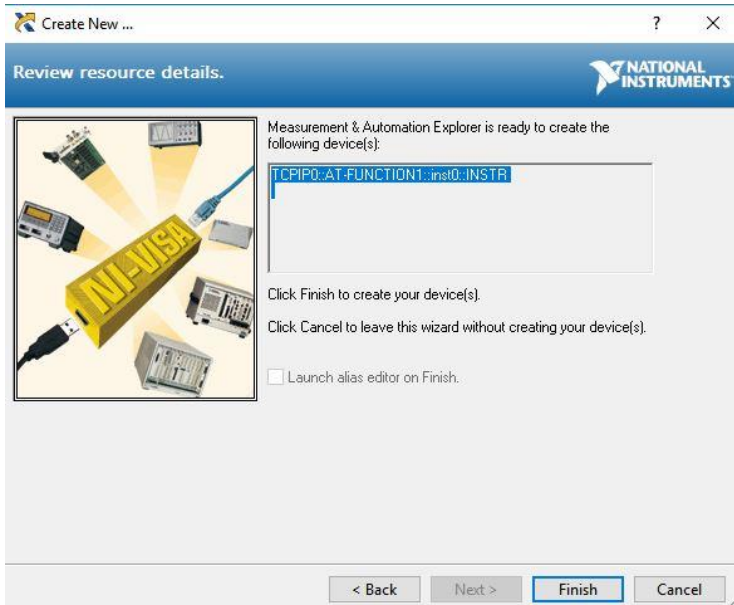

8. The AT-FUNCTION resource will be available in the Network Devices list

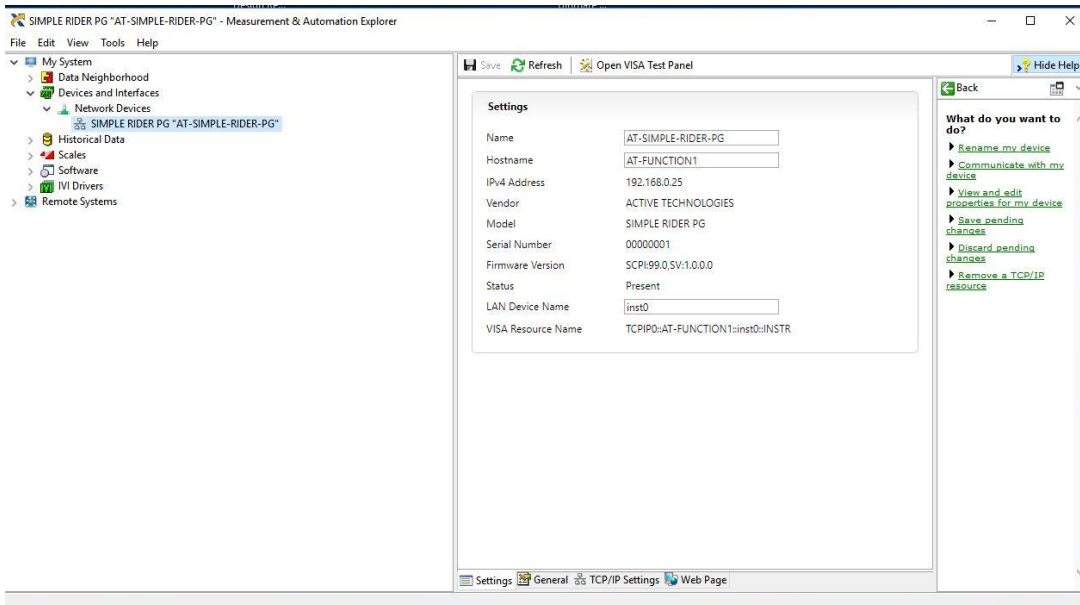


9. Now you can use send the SCPI commands to the AT-FUNCTION resource using the NI Visa Test Panel or the AT-Instrument-Communicator

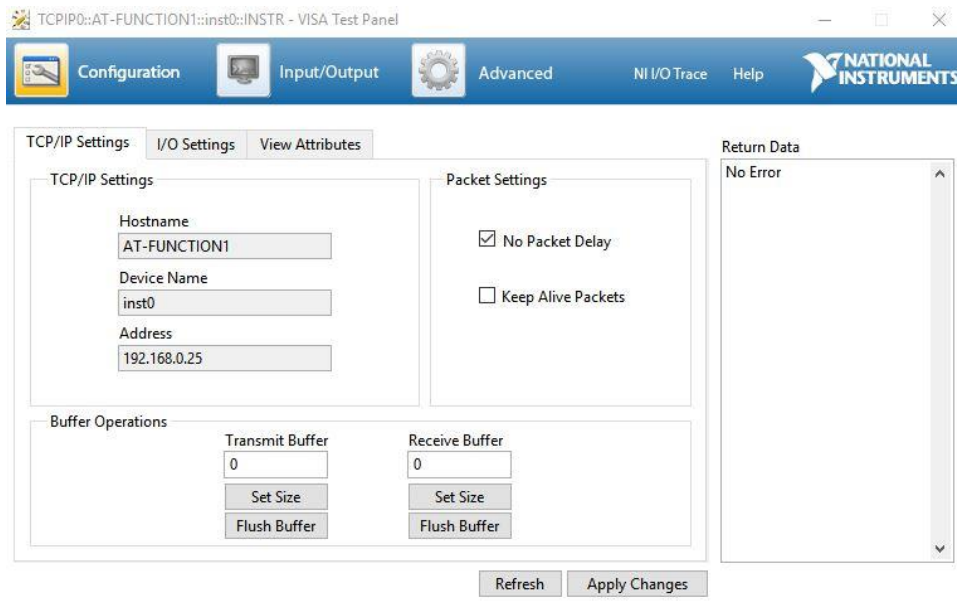

10. On the Client-PC (IP Address) or AWG instrument (LocalHost), launch the AT-Instrument-Communicator tool

### 4.1.1.1 AT Instrument Communicator

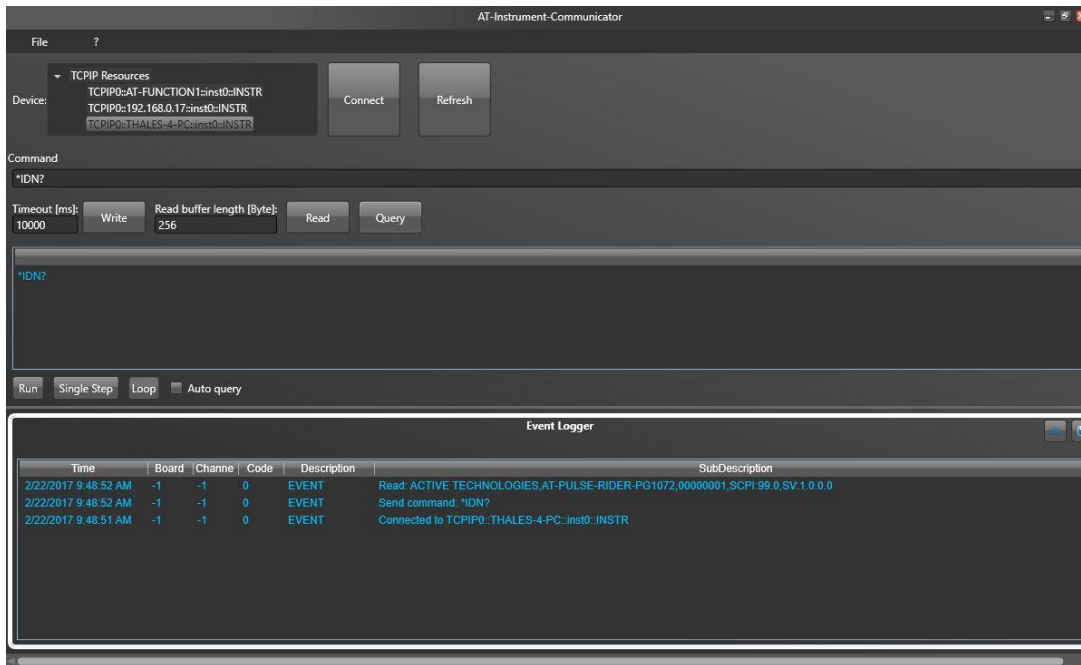

The AT-Instrument-Communicator software is a client-side component tool that uses NI-VISA on each remote PC, you must install a copy of NIVISA to make use of this client-side component (please follow the Prerequisite steps).

1. On the Client-PC launch the *AT Instrument Communicator* setup you can find in the folder “SDK\_SIMPLE\_RIDER\_AFG\_WEBSITE” and install the software.
2. Select the AT-FUNCTION resource on the Device list
3. Press the Connect button
4. If the instrument connection will be established, the SCPI command button will be enabled.
5. Write \*IDN? in the command
6. Press the Query button
7. In the Event Logger list, the instrument should respond like this: ACTIVE TECHNOLOGIES,AFG4012,T0302I000001,SCPI 99.0,SV 1.0.0 where T0302I000001 is the serial number, SCPI 99.0 is the SCPI command version and SV 1.0.0 is the Software Version.

8. A command script is a list of SCPI commands (one command for each line) saved in a txt file; you can send a command script using the File → Load Script menu item.

## 4.2 Command Groups

The following commands refer to the parameters [n] and [m] that depend on the instrument model.	<b>Parameter [n] = Available Channels</b>	<b>Parameter [m] = Available Marker Outputs</b>
Model 675-2C	1   2	1
Model 675-4C	1   2   3   4	1   2
Model 675-8C	1   2   3   4   5   6   7   8	1   2   3   4

**Table 12: Models and available parameters**

### Date and Time Commands

The date and time commands allow you to query the system date and time. The following table describes the date and time commands.

Command	Description
DATE	Query the system date
TIME	Query the system time

**Table 13: Date and Time Commands**

### 4.2.1 File System Commands

You can use the file commands to manipulate files and directories in the file system. The following table describes the file commands.

Command	Description
FILEsystem:CATalog?	Query the list of file and directory in the current working directory
FILEsystem:COpy	Copy a file from one location in the file system to another location
FILEsystem:CWDirectory	Change the current working directory in the file system
FILEsystem:DElete	Delete a file or directory in the file system

Command	Description
FILEsystem:HARDdisk?	Query the hard disk drive present on the instrument
FILEsystem:LOCK	Lock or unlock a file in the file system, or query if a file is locked
FILEsystem:MDIRectory	Create a directory in the file system
FILEsystem:UDISK?	Query the USB-disk drive connected to the instrument

**Table 14: File System Commands**

#### 4.2.2 Memory Commands

Memory commands let you manage the setup memory. The following table describes the memory commands.

Command	Description
MEMory:RECall	Recall a specified project file in the file system
MEMory:SAVE	Save the current project file in the file system
MEMory:STATE:DELeTe	Delete the setup memory
MEMory:STATE:LOCK	Lock or unlock the setup memory and query whether the memory is locked
MEMory:STATE:VALid?	Query the availability of setup memory
*RCL	Recall instrument settings from setup memory
*SAV	Save instrument settings to setup memory

**Table 15: Memory Commands**

#### 4.2.3 Mass Memory Commands

Mass memory commands let you change mass memory attributes. The following table describes the mass memory commands.



Command	Description
MMEMemory:LOAD:STATE	Copy a setup file to internal setup memory
MMEMemory:STORE:STATE	Copy a setup file from setup memory to a specified file in the file system

**Table 16: Mass Memory Commands**

#### 4.2.4 Output Commands

Output commands let you set output attributes. The following table describes the output commands.

Command	Description
OUTPut[n][:STATE]	Set or query the output state (on or off) on a specified channel
OUTPut[n]:IMPedance	Set or query the output load impedance
OUTPut[n]:POLarity	Set or query the polarity of the waveform on a specified channel
OUTPut[n]:LOW:IMPedance	Set or query the instrument output low impedance

**Table 17: Output Commands**

#### 4.2.5 Display Commands

Display commands let you to manage features related to the user interface.

Command	Description
HCOPY:SDUMp[:IMMEDIATE]	Create a screen shot of the display screen
DISPlay:CHANnel	Change the selected output page on the user interface

**Table 18: HCopy Command**

#### 4.2.6 Source Commands

Source commands let you set output waveform parameters. The following table describes the source commands.

Command	Description
[SOURce[n]]:AM[:DEPTH]	Set or query Amplitude Modulation depth
[SOURce[n]]:AM:INTernal:FREQuency	Set or query internal modulation frequency
[SOURce[n]]:AM:INTernal:FUNcTION	Set or query modulation waveform
[SOURce[n]]:AM:INTernal:FUNcTION:EFILe	Set or query a modulating waveform from file (EFILe)
[SOURce[n]]:AM:SOURce	Set or query the Amplitude Modulation source
[SOURce[n]]:AM:STATe	Enable or disable AM and query the state of AM
[SOURce[n]]:BURSt:MODE	Set or query the burst mode
[SOURce[n]]:BURSt:NCYCles	Set or query the burst count
[SOURce[n]]:BURSt[:STATe]	Enable or disable burst mode and query the burst mode
[SOURce[n]]:BURSt:TDELay	Set or query burst mode trigger delay time
[SOURce[n]]:COMBine:FEED	Set or query whether to add internal noise to an output signal for the specified channel
[SOURce[n]]:FM[:DEViation]	Set or query the peak frequency deviation

Command	Description
SOURce[n]:FM:INTernal:FREQuency	Set or query the internal modulation frequency
[SOURce[n]:FM:INTernal:FUNcTion	Set or query the internal modulation waveform
[SOURce[n]:FM:INTernal:FUNcTion:EFILe	Set or query the modulating waveform from file (EFILe)
[SOURce[n]:FM:SOURce	Set or query the frequency modulation source
[SOURce[n]:FM:STATe	Enable or disable Frequency Modulation and query the FM state
[SOURce[n]:FREQuency[:CW   :FIXed]	Set or query the output waveform frequency
[SOURce[n]:FREQuency:MODE	Set or query the frequency sweep state
[SOURce[n]:FREQuency:START	Set or query the sweep start frequency
[SOURce[n]:FREQuency:STOP	Set or query the sweep stop frequency
[SOURce[n]:FSKey[:FREQuency]	Set or query the FSK hop frequency
[SOURce[n]:FSKey:INTernal:RATE	Set or query the FSK internal modulation rate
[SOURce[n]:FSKey:SOURce	Set or query the FSK modulation source
[SOURce[n]:FSKey:STATe	Enable or disable FSK modulation and query the FSK modulation state
[SOURce[n]:PSKey[:FREQuency]	Set or query PSK modulation rate

Command	Description
[SOURce[n]]:PSKey:PHASe[:ADJust]	Set or query the PSK phase hop
[SOURce[n]]:PSKey: STATE	Enable or disable PSK modulation and query the FSK modulation state
[SOURce[n]]:PSKey:SOURce	Set or query PSK modulation source
[SOURce[n]]:FUNCTion:EFILe	Set or query the output waveform from file (EFILe)
[SOURce[n]]:FUNCTion:RAMP:SYMMetry	Set or query ramp waveform symmetry
[SOURce[n]]:FUNCTion[:SHAPE]	Set or query the shape of the carrier waveform
[SOURce[n]]:INITDELay	Set or query the initial delay
[SOURce[n]]:PHASe[:ADJust]	Set or query the output waveform phase
[SOURce[n]]:PM[:DEViation]	Set or query the peak phase deviation of phase modulation
[SOURce[n]]:PM:INTernal:FREQuency	Set or query the internal modulation frequency
[SOURce[n]]:PM:INTernal:FUNCTion	Set or query the internal modulation waveform
[SOURce[n]]:PM:INTernal:FUNCTion:EFILe	Set or query the PM modulating waveform from file(EFILe)
[SOURce[n]]:PM:SOURce	Set or query the Phase Modulation source
[SOURce[n]]:PM:STATE	Enable or disable PM modulation and query

Command	Description
	the PM modulation state
[SOURce[n]]:POWer[:LEVel][:IMMediate][:AMPLitude]	Set or query the internal noise level added to the output signal
[SOURce[n]]:PULSe:DCYCLe	Set or query the pulse waveform duty cycle
[SOURce[n]]:PULSe:PERiod	Set or query the pulse waveform period
[SOURce[n]]:PULSe:TRANSition[:LEADing]	Set or query the pulse waveform leading edge time
[SOURce[n]]:PULSe:TRANSition:TRAILing	Set or query the pulse waveform trailing edge time
[SOURce[n]]:PULSe:WIDTh	Set or query the pulse waveform width
[SOURce[n]]:PWM:INTernal:FREQuency	Set or query the Pulse Width Modulation frequency
[SOURce[n]]:PWM:INTernal:FUNcTION	Set or query the PWM modulating waveform
[SOURce[n]]:PWM:INTernal:FUNcTION:EFILe	Set or query the modulating waveform from file (EFILe)
[SOURce[n]]:PWM:SOURce	Set or query the Pulse Width Modulation source
[SOURce[n]]:PWM:STATe	Set or query the Pulse Width Modulation status
[SOURce[n]]:PWM[:DEViation]:DCYCLe	Set or query the Pulse Width Modulation deviation
[SOURce]:ROSCillator:SOURce	Set or query the clock reference input source

Command	Description
[SOURce]:ROSCillator:FREQuency	Set or query the clock reference input frequency
[SOURce[n]]:SWEep:HTIME	Set or query the sweep hold time
[SOURce[n]]:SWEep:MODE	Set or query the sweep mode
[SOURce[n]]:SWEep:NSTEP	Set or query the number of step of the upstairs sweep
[SOURce[n]]:SWEep:RTIME	Set or query the sweep return time
[SOURce[n]]:SWEep:SPACing	Set or query the sweep spacing
[SOURce[n]]:SWEep:SPACing:EFILe	Set or query the the sweep profile from file (EFILe)
[SOURce[n]]:SWEep:TIME	Set or query the sweep time
[SOURce[n]]:VOLTage:UNIT	Set or query the output amplitude units
[SOURce[n]]:VOLTage[:LEVel][:IMMediate]:HIGH	Set or query the output signal high level
[SOURce[n]]:VOLTage[:LEVel][:IMMediate]:LOW	Set or query the output signal low level
[SOURce[n]]:VOLTage[:LEVel][:IMMediate][:AMPLitude]	Set or query the output amplitude
[SOURce[n]]:VOLTage:VOCM	Set or query the DC common mode offset on the selected channel. The Common is 0V.
[SOURce[n]]:DOUBLEPULSe:PULSe[m]:AMPLitude	Set or query the amplitude of the first or of the second pulse of the double pulse waveform.

Command	Description
[SOURce[n]]:DOUBLEPULSe:PULSe[m]:TRANSition[:LEADing]	Set or query the leading edge of the first or of the second pulse of the double pulse waveform.
[SOURce[n]]:DOUBLEPULSe:PULSe[m]:TRANSition:TRAILing	Set or query the trailing edge of the first or of the second pulse of the double pulse waveform.
[SOURce[n]]:DOUBLEPULSe:PULSe[m]:WIDTh	Set or query the width of the first or of the second pulse of the double pulse waveform.
[SOURce[n]]:DOUBLEPULSe:PULSe[m]:DELay	Set or query the delay of the first or of the second pulse of the double pulse waveform.
[SOURce[n]]:COUPLE:STATe	Enable or disable the channel coupling
[SOURce[n]]:COUPLE:AMPLitude:STATe	Enable or disable the channel coupling for the amplitude parameter
[SOURce[n]]:COUPLE:AMPLitude:RATio	Set or query the ratio for the amplitude parameter in coupling mode
[SOURce[n]]:COUPLE:AMPLitude:OFFSet	Set or query the offset for the amplitude parameter in coupling mode
[SOURce[n]]:COUPLE:OFFSet:STATe	Enable or disable the channel coupling for the offset parameter

Command	Description
[SOURce[n]]:COUPLE:OFFSet:RATio	Set or query the ratio for the offset parameter in coupling mode
[SOURce[n]]:COUPLE:OFFSet:OFFSet	Set or query the offset for the offset parameter in coupling mode
[SOURce[n]]:COUPLE:FREQUency:STATe	Enable or disable the channel coupling for the frequency parameter
[SOURce[n]]:COUPLE:FREQUency:RATio	Set or query the ratio for the frequency parameter in coupling mode
[SOURce[n]]:COUPLE:FREQUency:OFFSet	Set or query the offset for the frequency parameter in coupling mode
[SOURce[n]]:COUPLE:PHASe:STATe	Enable or disable the channel coupling for the phase parameter
[SOURce[n]]:COUPLE:PHASe:RATio	Set or query the ratio for the phase parameter in coupling mode
[SOURce[n]]:COUPLE:PHASe:OFFSet	Set or query the offset for the amplitude parameter in coupling mode
[SOURce[n]]:COUPLE:DCYCLe:STATe	Enable or disable the channel coupling for the duty cycle parameter
[SOURce[n]]:COUPLE:DCYCLe:RATio	Set or query the ratio for the duty cycle



Command	Description
	parameter in coupling mode
[SOURce[n]]:COUPLE:DCYCLe:OFFSet	Set or query the offset for the duty cycle parameter in coupling mode
[SOURce[n]]:COUPLE:LEADIng:STATe	Enable or disable the channel coupling for the leading edge parameter
[SOURce[n]]:COUPLE:LEADIng:RATIo	Set or query the ratio for the leading edge parameter in coupling mode
[SOURce[n]]:COUPLE:LEADIng:OFFSet	Set or query the offset for the leading edge parameter in coupling mode
[SOURce[n]]:COUPLE:TRAIling:STATe	Enable or disable the channel coupling for the trailing edge parameter
[SOURce[n]]:COUPLE:TRAIling:RATIo	Set or query the ratio for the trailing edge parameter in coupling mode
[SOURce[n]]:COUPLE:TRAIling:OFFSet	Set or query the offset for the trailing edge parameter in coupling mode
[SOURce[n]]:COUPLE:SYMMetry:STATe	Enable or disable the channel coupling for the ramp symmetry parameter
[SOURce[n]]:COUPLE:SYMMetry:RATIo	Set or query the ratio for the ramp symmetry parameter in coupling mode

Command	Description
[SOURce[n]]:COUPLE:SYMMetry:OFFSet	Set or query the offset for the ramp symmetry parameter in coupling mode
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:AMPLitude:STATe	Enable or disable the channel coupling for the amplitude parameter of the double pulse waveform
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:AMPLitude:RATio	Set or query the ratio for the amplitude parameter of the double pulse waveform in coupling mode
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:AMPLitude:OFFSet	Set or query the offset for the amplitude parameter of the double pulse waveform in coupling mode
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:STATe	Enable or disable the channel coupling for the leading edge parameter of the double pulse waveform
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:RATio	Set or query the ratio for the leading edge parameter of the double pulse waveform in coupling mode
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:OFFSet	Set or query the offset for the leading edge parameter of the double pulse

Command	Description
	waveform in coupling mode
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:STATe	Enable or disable the channel coupling for the trailing edge parameter of the double pulse waveform
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:RATIo	Set or query the ratio for the trailing edge parameter of the double pulse waveform in coupling mode
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:OFFSet	Set or query the offset for the trailing edge parameter of the double pulse waveform in coupling mode
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:STATe	Enable or disable the channel coupling for the width parameter of the double pulse waveform
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:RATIo	Set or query the ratio for the width parameter of the double pulse waveform in coupling mode
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:OFFSet	Set or query the offset for the width parameter of the double pulse waveform in coupling mode

Command	Description
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:DELay:STATe	Enable or disable the channel coupling for the delay parameter of the double pulse waveform
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:DELay:RATio	Set or query the ratio for the delay parameter of the double pulse waveform in coupling mode
[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:DELay:OFFSet	Set or query the offset for the delay parameter of the double pulse waveform in coupling mode
[SOURce[n]]:VOLTage:LIMit:HIGH	Set or query the output amplitude upper limit
[SOURce[n]]:VOLTage:LIMit:LOW	Set or query the output amplitude lower limit

Table 19: Source Commands

#### 4.2.7 Device commands

Use the following commands to control the device:

Command	Description
AFGControl:START	Run the instrument
AFGControl:STOP	Stop the instrument
AFGControl:STATus	Return the status of the instrument
AFGControl:COPIY	Copies all parameter data from one channel to the other
AFGControl:AWGSwitch	Switches from AT-Simple-AFG to AT-True-ARB software

Table 20: Device Commands

#### 4.2.8 Status Commands

Status commands let you determine the status of the instrument. The following table describes the status commands

Command	Description
STATus:OPERation[:EVENT]?	Return the value in the Operation Event Register
STATus:OPERation:CONDition?	Return the contents of the Operation Condition Register
STATus:OPERation:ENABle	Set or query the mask for the Operation Enable Register
STATus:QUESTionable[:EVENT]?	Return the value in the Questionable Event Register
STATus:QUESTionable:CONDition?	Return the contents of the Questionable Condition Register
STATus:QUESTionable:ENABle	Set or query the mask for the Questionable Enable Register
STATus:PRESet	Preset SCPI Enable Register
*CLS	Clear all event registers and queue
*ESE	Set or query the Event Status Enable Register
*ESR?	Return the contents of the Standard Event Status Register
*SRE	Set or query the Service Request Enable Register
*STB?	Read the Status Byte Register

**Table 21: Status Commands**

#### 4.2.9 Synchronization Group Commands

Synchronization commands let you synchronize the operation of the instrument. The following table describes the synchronization commands.

Command	Description
*OPC	Set or query the operation complete message

*WAI	Wait to continue until pending commands complete
------	--

**Table 22: Synchronization group commands**

#### 4.2.10 System Group Commands

System commands let you control miscellaneous instrument functions. The following table describes the system commands.

Command	Description
*IDN?	Returns identification information for the instrument
*RST	Resets the instrument to its default state
SYSTem:BEEPper[:IMMediate]	Generate an audible tone
SYSTem:BEEPper:STATe	Set or query the beeper state
SYSTem:ERRor[:NEXT]?	Return the contents of the error event queue
SYSTem:KCLick[:STATe]	Enable or disable the key-click and user interface touch sound; query the status of key clicks
SYSTem:TLOCK[:STATe]	Lock or unlock the touch screen interface and query the lock state of the UI
SYSTem:ULANguage?	Query the language for the display screen
SYSTem:VERSion?	Return the SCPI conformance version information

**Table 23: System group commands**

#### 4.2.11 Trace Commands

Trace commands allow you to save, recall, set, and query data points in arbitrary buffer memory. The following table describes the trace commands.

TRACe[n][:DATA]	Send or return waveform data in the Arb Buffer of the selected channel
TRACe[n]:POINts	Query the number of points in the Arb Buffer for waveform data
TRACe[n]:SAVE	Save the contents of Arbitrary Buffer to a file in the system
TRACe[n]:RECall	Recall the contents of Arbitrary Buffer from a specific file in the file system

**Table 24: Trace group commands**

#### 4.2.12 Trigger Group Commands

The trigger commands let you control all aspects of triggering. The following table describes the trigger commands.

<b>Command</b>	<b>Description</b>
ABORt	Reset and initialize the trigger system
*TRG	Generates a trigger event
TRIGger[:SEQuence][:IMMediate]	Generates a trigger event
TRIGger[:SEQuence]:THREshold	Set or query the trigger threshold of an input signal
TRIGger[:SEQuence]:SLOPe	Set or query the slope of the trigger signal
TRIGger[:SEQuence]:SOURce	Set or query the source of the trigger signal
TRIGger[:SEQuence]:TIMer	Set or query the internal rate
TRIGger[:SEQuence]:IMPedance	Set or query the trigger input impedance
TRIGger[m]:OUTPut[:AMPLitude]	Set or query the marker out amplitude
TRIGger[m]:OUTPut:DELay	Set or query the skew of the marker out
TRIGger[m]:OUTPut:STATe	Enables or disables the marker out
TRIGger[m]:OUTPut:LINK	Links the marker out to an output channel

Table 25: Trigger group commands

### 4.3 COMMAND DESCRIPTIONS

<b>Command</b>	IDN (Query only)
<b>Description</b>	This command queries the instrument identifier.
<b>Group</b>	System
<b>Syntax</b>	*IDN?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<p>&lt;Manufacturer&gt;,&lt;Model&gt;,&lt;Serial Number&gt;,&lt;SCPI Version&gt;,&lt;Firmware Version&gt;            Where:            &lt;Manufacturer&gt;::= ACTIVE TECHNOLOGIES            &lt;Model&gt;::=AFG4012            &lt;Serial Number&gt;::=indicates an actual serial number)            &lt;SCPI Version&gt;::=SCPI:99.0 FV:1.0            &lt;Software Version&gt;::=SV: 1.0.0 (1.0.0. is system software version)</p>
<b>Example</b>	<p>*IDN?            Example return:            ACTIVE TECHNOLOGIES,AFG4012,T0302I000001,SCPI:99.0,SV:1.0.0</p>

<b>Command</b>	DATE (Query only)
<b>Description</b>	This command queries the system date.
<b>Group</b>	Date and Time
<b>Syntax</b>	DATE?
<b>Related Commands</b>	TIME
<b>Arguments</b>	None
<b>Returns</b>	<date_string>::<string> Returns a date in the format "DATE yyyy-mm-dd".
<b>Example</b>	DATE? Example return: "DATE 2018-01-13," which means the system date is January 13th, 2018.



**Table 26: DATE**

<b>Command</b>	TIME (Query only)
<b>Description</b>	This command queries the system time.
<b>Group</b>	Date and Time
<b>Syntax</b>	TIME?
<b>Related Commands</b>	DATE
<b>Arguments</b>	None
<b>Returns</b>	<time_string>::=<string> returns the current system time in the format "TIME hh:mm:ss".
<b>Example</b>	TIME? Example return: "TIME 12:25:30"

**Table 27: TIME**

<b>Command</b>	FILEsystem:CATalog (Query only)
<b>Description</b>	This command returns the list of all file and directory contained in the Current Working Directory. This command is query only.
<b>Group</b>	File System
<b>Syntax</b>	FILESystem:CATalog?
<b>Related Commands</b>	FILEsystem:CWDirectory
<b>Arguments</b>	None
<b>Returns</b>	<NR1>,<NR1>[,<file_name>,<file_type>,<file_size>]... Where: The first <NR1> indicates the total amount of storage currently used, in bytes. The second <NR1> indicates the available free space in storage, in bytes. <file_name> is the exact name of a file. <file_type> is DIR for directory, otherwise it is blank. <file_size> is the size of the file, in bytes.
<b>Example</b>	FILESystem:CATalog? Example return: 32751616,27970560,"SAMPLE1.afs,,5412"

**Table 28: FILEsystem:CATalog**

<b>Command</b>	FILEsystem:COPY
<b>Description</b>	This command copies a file in the file system to another file in the file system. This command causes an error if filename1 (source file) in the file system doesn't exist, if filename2 (destination file) is locked, or if the destination directory is locked. The allowed file extensions are ".txt", ".afs", ".bmp". There is no query form of this command.
<b>Group</b>	File System

<b>Syntax</b>	FILEsystem:COPY <filename1>,<filename2>
<b>Related Commands</b>	FILEsystem:LOCK FILEsystem:DELeTe FILEsystem:CWDirectory
<b>Arguments</b>	<filename1>::=<Qstring> specifies a source file name in the instrument file system. <filename2>::=<Qstring> specifies a destination file name in the instrument file system. You can insert absolute or relative path: if the path is relative, it starts from the Current Working Directory.
<b>Returns</b>	None
<b>Example</b>	FILEsystem:COPY "SAMPLE1.afs","SAMPLE2.afs" Copies the file named "SAMPLE1.afs" to the file "SAMPLE2.afs" in the Current Working Directory.

**Table 29: FILEsystem:COPY**

<b>Command</b>	FILEsystem:CWDirectory
<b>Description</b>	This command changes or queries the current working directory in the instrument file system.
<b>Group</b>	File System
<b>Syntax</b>	FILEsystem:CWDirectory <directory_path> FILEsystem:CWDirectory?
<b>Related Commands</b>	FILEsystem:LOCK FILEsystem:DELeTe
<b>Arguments</b>	<directory_name>::=<Qstring> indicates the working directory in the file system that you want to change. The default value is: "C:\Users\Arb Rider\AppData\Roaming\Active Technologies\AT-FUNCTION-RIDER\AWG3352\"
<b>Returns</b>	<directory_name>::=<Qstring>
<b>Example</b>	FILEsystem:CWDirectory "C:\Users" Change the current directory to C:\Users.

**Table 30: FILEsystem:CWDirectory**

<b>Command</b>	FILEsystem:DELeTe
<b>Description</b>	This command deletes a file or directory from the file system. If a specified file in file storage locked and cannot be deleted, this command causes an error. The allowed file extensions are ".txt",

	".afs", ".bmp". You can delete a directory if it is empty. There is no query form of this command.
<b>Group</b>	File System
<b>Syntax</b>	FILEsystem:DElete <file_name>
<b>Related Commands</b>	FILEsystem:CWDirectory MEMory:SAVE
<b>Arguments</b>	<file_name>::=<Qstring> specifies a file to be deleted. You can insert absolute or relative path: if the path is relative, it starts from the Current Working Directory.
<b>Return</b>	None
<b>Example</b>	FILEsystem:DElete "SETUP1.afs" Delete the file " SETUP1.afs" in the current working directory of the file system.

**Table 31: FILEsystem:DElete**

<b>Command</b>	FILEsystem:HARDdisk (Query only)
<b>Description</b>	This command queries the hard disk drive. This command is query only.
<b>Group</b>	File System
<b>Syntax</b>	FILEsystem:HARDdisk?
<b>Related Commands</b>	FILEsystem:UDISK?
<b>Arguments</b>	None
<b>Return</b>	<driver1;driver2;driver3...>
<b>Example</b>	FILEsystem:HARDdisk? Example return: "C:\;D:\;E:\;F:\"

**Table 32: FILEsystem:HARDdisk**

<b>Command</b>	FILEsystem:LOCK
<b>Description</b>	This command sets or queries whether to lock a file in the file system. If you lock a file, you cannot overwrite or delete it. The allowed file extensions are ".txt", ".afs", ".bmp".
<b>Group</b>	File System
<b>Syntax</b>	FILEsystem:LOCK <file_name>, {ON   OFF   0   1} FILEsystem:LOCK? <file_name>
<b>Related Commands</b>	FILEsystem:CWDirectory
<b>Arguments</b>	<file_name> ::= Qstring, the file to lock, unlock or query the lock state. ON or 1 locks the specified file in the file system. OFF or 0 allows you to overwrite or delete a file or directory in the file system

<b>Return</b>	<NR1> 0 means that the selected memory is not locked, 1 means that it is locked.
<b>Example</b>	FILEsystem:LOCK "SETUP1.afs",ON Lock the file "SETUP1.afs".

**Table 33: FILEsystem:LOCK**

<b>Command</b>	FILEsystem:MDIRectory
<b>Description</b>	This command creates a directory in the file system. Note that the process is iterative, then it can create directory and subdirectories. There is no query form of this command.
<b>Group</b>	File System
<b>Syntax</b>	FILEsystem:MDIRectory <directory_name>
<b>Related Commands</b>	None
<b>Arguments</b>	<directory_name>::=<Qstring> specifies a directory name to be created. The path can be absolute or relative, if you insert a relative path it starts from Current Working Directory.
<b>Return</b>	None
<b>Example</b>	FILEsystem:MDIRectory "SAMPLE1" Create a directory named "SAMPLE1" in the Current Working Directory.

**Table 34: FILEsystem:MDIRectory**

<b>Command</b>	FILEsystem:UDISK? (Query only)
<b>Description</b>	This command queries the USB-disk drive. This command is query only.
<b>Group</b>	File System
<b>Syntax</b>	FILEsystem:UDISK?
<b>Related Commands</b>	FILEsystem:HARDdisk?
<b>Arguments</b>	None
<b>Return</b>	<driver1;driver2;driver3...>
<b>Example</b>	FILEsystem:UDISK? Example return: "G:\;H:\;"

**Table 35: FILEsystem:UDISK?**

<b>Command</b>	MEMory:RECall
<b>Description</b>	This command recalls a project file from a specified file in the file system to the current project. If the specified file does not exist or its

	format is wrong, this command causes an error. There is no query form of this command.
<b>Group</b>	Memory
<b>Syntax</b>	MEMory:RECall <file_name>
<b>Related Commands</b>	MEMory:SAVE
<b>Arguments</b>	<file_name>::=<Qstring> specifies a setup file to recall. The file path can be absolute or relative, if you insert a relative path it starts from Current Working Directory.
<b>Returns</b>	None
<b>Example</b>	MEMory:RECall "SETUP1.afs" Recalls a file in file storage named SETUP1.afs into the current project.

**Table 36: MEMory:RECall**

<b>Command</b>	MEMory:SAVE
<b>Description</b>	This command saves the current project file to a specified file in the file system. If the specified file in the file system is locked, this command causes an error. You cannot create a new file if the directory is locked. There is no query form of this command.
<b>Group</b>	Memory
<b>Syntax</b>	MEMory:SAVE <file_name>
<b>Related Commands</b>	MEMory:RECall
<b>Arguments</b>	<file_name>::=<Qstring> specifies a file name in the file system. The file path can be absolute or relative, if you insert a relative path it starts from Current Working Directory.
<b>Returns</b>	None
<b>Example</b>	MEMory:SAVE "SETUP1 " Copies the current project file to a file named "SETUP1 " in the file system.

**Table 37: MEMory:SAVE**

<b>Command</b>	MEMory:STAtE:DELeTe
<b>Description</b>	This command deletes the contents of specified setup memory. If the specified setup memory is locked and cannot be deleted, this command causes an error. There is no query form of this command.
<b>Group</b>	Memory
<b>Syntax</b>	MEMory:STAtE:DELeTe {0   1   2   3   4}
<b>Related Commands</b>	*SAV *RCL

	MEMory:STAtE:LOCK
<b>Arguments</b>	{0   1   2   3   4} specifies the location of setup memory.
<b>Returns</b>	None
<b>Example</b>	MEMory:STAtE:DELeTe 1 Delete the contents of the setup memory 1.

**Table 38: MEMory:STAtE:DELeTe**

<b>Command</b>	MEMory:STAtE:LOCK
<b>Description</b>	This command locks or unlocks the specified setup memory. If you lock a setup memory, you cannot overwrite or delete it. You cannot execute this command for the setup memory of location numbered + 0 (last setup memory). If a setup memory is not valid the command returns an error, but the query is allowed. The query form of this command returns the lock state of the setup memory.
<b>Group</b>	Memory
<b>Syntax</b>	MEMory:STAtE:LOCK {1   2   3   4},{ON   OFF   0   1} MEMory:STAtE:LOCK? {1   2   3   4}
<b>Related Commands</b>	None
<b>Arguments</b>	ON   1 locks the specified location of setup memory, OFF   0 allows you to overwrite or delete the specified location of setup memory.
<b>Returns</b>	<NR1> 0 means that the selected memory is not locked, 1 means that it is locked.
<b>Example</b>	MEMory:STAtE:LOCK 1,ON Lock the setup memory of location number 1

**Table 39: MEMory:STAtE:LOCK**

<b>Command</b>	MEMory:STAtE:VALid? (Query only)
<b>Description</b>	This command returns the availability of a setup memory. This command is query only.
<b>Group</b>	Memory
<b>Syntax</b>	MEMory:STAtE:VALid? {0   1   2   3   4}
<b>Related Commands</b>	None
<b>Arguments</b>	{0   1   2   3   4} specifies the location of setup memory.
<b>Returns</b>	<NR1> 1 means that the specified setup memory has been saved. 0 means that the specified setup memory has been deleted.

<b>Example</b>	MEMory:STATe:VALid? 0 Example return: 1, means that the setup memory 0 has been saved.
----------------	---

**Table 40: MEMory:STATe:VALid?**

<b>Command</b>	*RCL
<b>Description</b>	This command restores the state of the instrument from a copy of the settings stored in the setup memory. If the specified setup memory is deleted, this command causes an error. The setup memory location numbered 0 contains the last settings saved when you power of the instrument. There is no query form of this command.
<b>Group</b>	Memory
<b>Syntax</b>	*RCL {0   1   2   3   4}
<b>Related Commands</b>	*SAV
<b>Arguments</b>	{0   1   2   3   4} specifies the location of the setup memory.
<b>Returns</b>	None
<b>Example</b>	*RCL 3 Restores the instrument settings from a copy of the settings stored in memory location 3.

**Table 41: \*RCL**

<b>Command</b>	*SAV
<b>Description</b>	This command stores the current settings of the Arbitrary Function Generator to a specified setup memory location. If the memory location is already valid it will be overwritten. The setup memory location numbered 0 (last setup memory) is automatically overwritten with the current settings when you power off the instrument. If the specified number setup memory is locked, this command causes an error. There is no query form of this command.
<b>Group</b>	Memory
<b>Syntax</b>	*SAV {0   1   2   3   4}
<b>Related Commands</b>	*RCL
<b>Arguments</b>	{0   1   2   3   4} specifies the location of setup memory.
<b>Returns</b>	None
<b>Example</b>	*SAV 2 Save the current instrument state in the memory location 2

**Table 42: \*SAV**

<b>Command</b>	HCOPY:SDUMp[:IMMediate]
----------------	-------------------------

<b>Description</b>	This command copies the current screen shot to a file in the file system. The file will be named with the format "year-month-day-hour-minus-seconds.bmp" in the system folder: "C:\Screenshots\". There is no query form of this command.
<b>Group</b>	HCOPY
<b>Syntax</b>	HCOPY:SDUMp[:IMMEDIATE]
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	HCOPY:SDUMp Copy the screen shot to the "C:\Screenshots\" system folder.

**Table 43: HCOPY:SDUMp[:IMMEDIATE]**

<b>Command</b>	DISPlay:CHANnel
<b>Description</b>	This command selects the user interface output channel page. There is no query form of this command.
<b>Group</b>	Display
<b>Syntax</b>	DISPlay:CHANnel {OUT1   OUT2   OUT3   OUT4   OUT5   OUT6   OUT7   OUT8 }
<b>Related Commands</b>	None
<b>Arguments</b>	<channel>:={OUT1   OUT2   OUT3   OUT4   OUT5   OUT6   OUT7   OUT8 } Note: <channel> string depends on the instrument model
<b>Returns</b>	None
<b>Example</b>	DISPlay:CHANnel OUT2 The user interface displays the output2 page.

**Table 44: DISPlay:CHANnel**

<b>Command</b>	MMEMemory:LOAD:STATe
<b>Description</b>	This command copies a setup file in the file system to an internal setup memory location. If the memory location is already valid it will be overwritten. If a specified internal setup memory is locked, this command causes an error. When you power-off the instrument, the memory location 0 is automatically overwritten with the current instrument setup. There is no query form of this command.
<b>Group</b>	Mass Memory
<b>Syntax</b>	MMEMemory:LOAD:STATe {0   1   2   3   4},<file_name>
<b>Related Commands</b>	MEMory:STATe:LOCK MMEMemory:STORE:STATe



<b>Arguments</b>	{0 1 2 3 4} specifies the location of setup memory. <file_name>::=<Qstring> specifies a setup file to be copied. The file path can be absolute or relative, if you insert a relative path it starts from Current Working Directory.
<b>Returns</b>	None
<b>Example</b>	MMEMemory:LOAD:STATe 1,"SETUP1.afs" Copies a file named SETUP1.afs in the file system into the internal memory location 1

**Table 45: MMEMemory:LOAD:STATe**

<b>Command</b>	MMEMemory:STORe:STATe
<b>Description</b>	This command copies a setup memory location to a specified file in the file system. If the file already exists it will be overwritten. If the specified file in the file system is locked, this command causes an error. You cannot create a new file if the directory is locked. If the setup memory is deleted, this command causes an error. <file_name> is a quoted string that defines the file name and path. There is no query form of this command.
<b>Group</b>	Mass Memory
<b>Syntax</b>	MMEMemory:STORe:STATe {0 1 2 3 4},<file_name>
<b>Related Commands</b>	MMEMemory:LOAD:STATe MEMemory:STATe:LOCK
<b>Arguments</b>	{0 1 2 3 4} specifies the location of setup memory. <file_name>::=<Qstring> specifies a file name in the file system. The file path can be absolute or relative, if you insert a relative path it starts from Current Working Directory.
<b>Returns</b>	None
<b>Example</b>	MMEMemory:STORe:STATe 1,"SETUP1.afs" Copies the setup in the setup memory location 1 to a file named "SETUP1.afs" in the Current Working Directory.

**Table 46: MMEMemory:STORe:STATe**

<b>Command</b>	OUTPut[n][:STATe]
<b>Description</b>	This command enables or disables the output for the specified channel. The query form of this command returns the output state of the channel.
<b>Group</b>	Output
<b>Syntax</b>	OUTPut[n][:STATe] {ON OFF 0 1} OUTPut[n][:STATe]?

<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. ON   1 enables the arbitrary function generator output. OFF   0 disables the arbitrary function generator output.
<b>Returns</b>	<NR1> 1 means that the output is enabled. 0 means that the output is disabled.
<b>Example</b>	OUTPut1:STATe ON Set the arbitrary function generator output channel 1 (OUT 1) to ON.

**Table 47: OUTPut[n]::STATe]**

<b>Command</b>	OUTPut[n]:IMPedance
<b>Description</b>	This command sets the output load impedance for the specified channel. The specified value is used for amplitude, offset, and high/low level settings. You can set the impedance to any value from 1 Ω to 1 MΩ. The default value is 50 Ω. The query form of this command returns the current set impedance, minimum or maximum load impedance setting in ohms.
<b>Group</b>	Output
<b>Syntax</b>	The value of n indicates the channel number. OUTPut[n]:IMPedance <ohms> OUTPut[n]:IMPedance? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <ohms>::=< NR1 >[<units>] Where: <units>::=OHM is the value of the load impedance in ohms
<b>Returns</b>	<ohms>::=<NR1>
<b>Example</b>	OUTPut1:IMPedance 60 Set the channel 1 (CH 1) load impedance to 60 Ohm.

**Table 48: OUTPut[n]:IMPedance**

<b>Command</b>	OUTPut[n]:LOW:IMPedance
<b>Description</b>	This command sets the instrument impedance to low (5 Ohm) that means the output is short-circuited using a relay. If the output impedance is set to false, the instrument impedance is set to 50 Ohm (default).

	The query form of this command returns the instrument impedance.
<b>Group</b>	Output
<b>Syntax</b>	The value of n indicates the channel number. ON   1 sets the instrument impedance to 5 Ohm. OFF   0 sets the instrument impedance to 50 Ohm.
<b>Related Commands</b>	None
<b>Arguments</b>	<NR1> 1 means that the instrument impedance is set to Low (50hm) 0 means that the instrument impedance is set to 50 Ohm
<b>Returns</b>	<ohms>::=<NR1>
<b>Example</b>	OUTPut1:LOW:IMPedance ON sets the instrument impedance to Low.

**Table 49: OUTPut[n]:LOW:IMPedance**

<b>Command</b>	OUTPut[n]:POLarity
<b>Description</b>	This command inverts the output waveform relative to the zero level. The query form of this command returns the polarity for the specified channel.
<b>Group</b>	Output
<b>Syntax</b>	OUTPut[n]:POLarity {NORMAL   INVERTed} OUTPut[n]:POLarity?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. NORMAL sets the specified output waveform polarity to Normal. INVERTed sets the specified output waveform polarity to Inverted.
<b>Returns</b>	<NR1> 0 means the polarity is normal, 1 means the polarity is inverted.
<b>Example</b>	OUTPut1:POLarity NORMAL Set the channel 1 (CH 1) waveform polarity to Normal.

**Table 50: OUTPut[n]:POLarity**

<b>Command</b>	[SOURce[n]]:AM[:DEPTH]
<b>Description</b>	This command sets or queries the AM modulation depth for the specified channel. This command and this query will cause an error if it is not in the AM modulation state.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:AM:DEPTH <depth> [SOURce[n]]:AM:DEPTH? [MINimum   MAXimum]

<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <depth>::=<NR2>[<units>] Where: <NR2> is the depth of modulating frequency. <units>::=PCT MINimum queries the modulation depth minimum value. MAXimum queries the modulation depth maximum value.
<b>Returns</b>	<depth>
<b>Example</b>	SOURce1:AM:DEPth 70 Set the depth of the modulating signal on channel (CH 1) to 70%

**Table 51: [SOURce[n]]:AM[:DEPth]**

<b>Command</b>	[SOURce[n]]:AM:INTernal:FREQuency
<b>Description</b>	This command sets or queries the internal AM modulation frequency for the specified channel. This command will cause an error if it is not in the AM modulation state.
<b>Group</b>	Source
<b>Syntax</b>	The value of n indicates the channel number. [SOURce[n]]:AM:INTernal:FREQuency <frequency> [SOURce[n]]:AM:INTernal:FREQuency? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:AM:SOURce
<b>Arguments</b>	The value of n indicates the channel number. <frequency>::=<NRf>[<units>] Where: <NRf> is the modulation frequency. <units>::=[Hz   kHz   MHz]. MINimum queries the modulation frequency minimum value. MAXimum queries the modulation frequency maximum value.
<b>Returns</b>	<frequency>
<b>Example</b>	SOURce1:AM:INTernal:FREQuency 10kHz Set the channel 1 (CH 1) internal modulation frequency to 10 kHz.

**Table 52: [SOURce[n]]:AM:INTernal:FREQuency**

<b>Command</b>	[SOURce[n]]:AM:INTernal:FUNCTion
<b>Description</b>	This command sets or queries the AM modulating waveform for the specified channel. You can use this command only when the internal modulation source is selected. If you specify EFILE when there is no EFILE or the EFILE is not yet defined, this command causes an error. This command and this query will cause an error if

	not in the AM modulation state. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:AM:INTernal:FUNctIon {SINusoid   SQUare   TRIangle   RAMP   NRAMp   PRNoise   ARBB   EFILE} [SOURce[n]]:AM:INTernal:FUNctIon?
<b>Related Commands</b>	[SOURce[n]]:AM:SOURce
<b>Arguments</b>	The value of n indicates the channel number. SINusoid   SQUare   TRIangle   RAMP   NRAMp   PRNoise One of six types of function waveform can be selected as a modulating signal. ARBB   EFILE can be selected as a modulating file.
<b>Returns</b>	SIN   SQU   TRI   RAMP   NRAM   PRN   ARBB   EFILE
<b>Example</b>	SOURce1:AM:INTernal:FUNctIon SQUare Select square as the shape of modulating waveform for the channel 1 (CH 1) output

**Table 53: [SOURce[n]]:AM:INTernal:FUNctIon**

<b>Command</b>	[SOURce[n]]:AM:INTernal:FUNctIon:EFILE
<b>Description</b>	This command sets or queries the EFILE name used as a modulating waveform for AM modulation. A file name must be specified in the file system, the valid file extensions are ".txt", ".csv" and ".trc". If the file is not set the query returns "". If the file contains more than 16834 samples, it will be decimated. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	The value of n indicates the channel number. [SOURce[n]]:AM:INTernal:FUNctIon:EFILE <file_name> [SOURce[n]]:AM:INTernal:FUNctIon:EFILE?
<b>Related Commands</b>	FILEsystem:CWDirectory
<b>Arguments</b>	The value of n indicates the channel number. <file_name>::=<Qstring> specifies a file name in the file system. The <file_name> includes the path. The path can be absolute or relative, if you insert a relative path it starts from Current Working Directory.
<b>Returns</b>	<file_path>
<b>Example</b>	SOURce1:AM:INTernal:FUNctIon:EFILE "SAMPLE1.txt" Sets a file named "SAMPLE1" in the Current Working Directory of the file system.

**Table 54: [SOURCE[n]]:AM:INTERNAL:FUNCTION:EFILE**

<b>Command</b>	[SOURCE[n]]:AM:SOURce
<b>Description</b>	This command sets or queries the source of the AM modulating signal for the specified channel. This command will cause an error if not in the AM modulation state.
<b>Group</b>	Source
<b>Syntax</b>	The value of n indicates the channel number. [[SOURCE[n]]:AM:SOURce [INTERNAL   EXTERNAL] [SOURCE[n]]:AM:SOURce?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. INTERNAL means that the carrier waveform is modulated with an internal function. EXTERNAL means that the carrier waveform is modulated with an external source.
<b>Returns</b>	INT   EXT
<b>Example</b>	SOURCE1:AM:SOURce INTERNAL Set the channel 1 (CH 1) source of the modulating signal to internal.

**Table 55: [SOURCE[n]]:AM:SOURce**

<b>Command</b>	[SOURCE[n]]:AM:STATe
<b>Description</b>	This command enables or disables AM modulation for the specified channel. The query version of this command returns the state of AM modulation. When you send this command and the state changes, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURCE[n]]:AM:STATe { ON   OFF   0   1 } [SOURCE[n]]:AM:STATe?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. ON   1 enables AM modulation. OFF   0 disables AM modulation.
<b>Returns</b>	<NR1> 0 means OFF, 1 means ON
<b>Example</b>	SOURCE1:AM:STATe ON Enable the channel 1 (CH 1) AM modulation.

**Table 56: [SOURCE[n]]:AM:STATe**

<b>Command</b>	[SOURce[n]]:BURSt:MODE
<b>Description</b>	This command sets or queries the burst mode for the specified channel. This command will cause an error if not in the BURST state. When you change the burst mode from gated to triggered, by default it set a burst of N cycles, where N is the last number of cycles. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:BURSt:MODE {TRIGgered   GATed} [SOURce[n]]:BURSt:MODE?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. TRIGgered means that triggered mode is selected for the burst mode. GATed means that gated mode is selected for the burst mode.
<b>Returns</b>	TRIG   GAT
<b>Example</b>	SOURce1:BURSt:MODE TRIGgered Selects the triggered mode.

**Table 57: [SOURce[n]]:BURSt:MODE**

<b>Command</b>	[SOURce[n]]:BURSt:NCYCles
<b>Description</b>	This command sets or queries the number of cycles (burst count) to be output in burst mode for the specified channel. The query version of this command returns a number or INF if the burst count is set to INFinity. This command will cause an error if not in BURST state. Is not possible modify the number of cycles while the instrument is running, if this command is sent during the running mode an error occurs.
<b>Group</b>	Source
<b>Syntax</b>	The value of n indicates the channel number. [SOURce[n]]:BURSt:NCYCles {<cycles>   INFinity   MINimum   MAXimum} [SOURce[n]]:BURSt:NCYCles? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	<cycles>::=<NR1> Where: <NR1> is the burst count. The value of n indicates the channel number. The burst count ranges from 1 to 4,294,967,294.

	INFINITY sets the burst count to infinite. MINimum queries or sets the minimum count. MAXimum queries or sets the maximum count.
<b>Returns</b>	<cycles>
<b>Example</b>	SOURCE1:BURST:NCYCLES 2 Sets the channel 1 (CH 1) burst count to 2.

**Table 58: [SOURCE[n]]:BURST:NCYCLES**

<b>Command</b>	[SOURCE[n]]:BURST[:STATE]
<b>Description</b>	This command enables or disables the burst mode for the specified channel. The query version of this command returns the state of burst mode. When you send this command and the state changes, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURCE[n]]:BURST:STATE { ON   OFF   0   1 } [SOURCE[n]]:BURST:STATE?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. ON   1 enables the burst mode. OFF   disables the burst mode.
<b>Returns</b>	<NR1> 0 means OFF, 1 means ON
<b>Example</b>	SOURCE1:BURST:STATE ON Enable the burst mode for channel 1 (CH 1).

**Table 59: [SOURCE[n]]:BURST:STATE**

<b>Command</b>	[SOURCE[n]]:BURST:TDELAY
<b>Description</b>	This command sets or queries delay time in the burst mode for the specified channel. It specifies a time delay between the trigger and the signal output. This command is available only in the triggered burst mode. This command will cause an error if not in the BURST state. If you change the delay while the instrument is running, the burst is reset and the voltage level will be move to the offset level, instead of wait on the last sample. When you send this command, if the instrument is running it will be stopped. NOTE: this command changes the initial delay of the channel for all the run mode.
<b>Group</b>	Source



<b>Syntax</b>	[SOURce[n]]:BURSt:TDElay <delay> } [SOURce[n]]:BURSt:TDElay?[MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[1   2]]:INITDElay
<b>Arguments</b>	The value of n indicates the channel number. <delay>::=<NRf><units> Where: <units>::=[s   ms   μs   ns] MINimum queries the minimum delay. MAXimum queries the maximum delay.
<b>Returns</b>	<delay>
<b>Example</b>	SOURce1:BURSt:TDElay 20ms Set the channel 1 (CH 1) delay time to 20 ms

**Table 60: [SOURce[n]]:BURSt:TDElay**

<b>Command</b>	[SOURce[n]]:COMBine:FEED
<b>Description</b>	This command sets or queries whether to add the internal noise to the output signal for the specified channel. When you specify the internal noise, you can set or query the noise level by using the [SOURce[n]]:POWER[:LEVel][:IMMediate][:AMPLitude] command. To disable the internal noise function, specify "". If the carrier is Noise, this command causes an error.
<b>Group</b>	Source
<b>Syntax</b>	The value of n indicates the channel number. [SOURce[n]]:COMBine:FEED {"NOISe"   ""} [SOURce[n]]:COMBine:FEED?
<b>Related Commands</b>	[SOURce[n]]:POWER[:LEVel][:IMMediate][:AMPLitude]
<b>Arguments</b>	The value of n indicates the channel number. NOISe indicates that the internal noise is added to the output signal. "" disables the internal noise function.
<b>Returns</b>	"NOIS"   ""
<b>Example</b>	SOURce1:COMBine:FEED "NOISe" Add a noise signal to the channel 1 (CH 1) output signal.

**Table 61: [SOURce[n]]:COMBine:FEED**

<b>Command</b>	[SOURce[n]]:FM[:DEVIation]
<b>Description</b>	This command sets or queries the peak frequency deviation of FM modulation for the specified channel. The range of the frequency deviation setting depends on the waveform selected as the carrier and on its frequency. This command will cause an error if not in the

	frequency modulation state. When you send this command and the state changes, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	The value of n indicates the channel number. [SOURce[n]]:FM:DEVIation <deviation> [SOURce[n]]:FM:DEVIation?[MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	<deviation>::=<NRf>[<units>] Where: <NRf> is the frequency deviation. <units>::=[Hz   kHz   MHz] MINimum queries the minimum deviation. MAXimum queries the maximum deviation.
<b>Returns</b>	<deviation>
<b>Example</b>	SOURce1:FM:DEVIation 1.0MHz Set the channel 1 (CH 1) frequency deviation to 1.0 MHz.

**Table 62: [SOURce[n]]:FM[:DEVIation]**

<b>Command</b>	[SOURce[n]]:FM:INTernal:FREQuency
<b>Description</b>	This command sets or queries the internal modulation frequency of FM modulation for the specified channel. This command will cause an error if not in frequency modulation state.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FM:INTernal:FREQuency <frequency> [SOURce[n]]:FM:INTernal:FREQuency?[MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <frequency>::=<NRf>[<units>] Where: <NRf> is the modulation frequency. <units>::=[Hz   kHz   MHz] MINimum queries the minimum frequency. MAXimum queries the maximum frequency.
<b>Returns</b>	<frequency>
<b>Example</b>	SOURce1:FM:INTernal:FREQuency 10kHz Set the channel 1 (CH 1) internal modulation frequency to 10 kHz.

**Table 63: [SOURce[n]]:FM:INTernal:FREQuency**

<b>Command</b>	[SOURce[n]]:FM:INTernal:FUNCTion
<b>Description</b>	This command sets or queries the FM modulating waveform for the specified channel. You can use this command only when the internal modulation source is selected. If you specify EFILE when there is no

	EFILe or the EFILe is not yet defined, this command causes an error. This command will cause an error if not in the frequency modulation state. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FM:INTernal:FUNCTion {SINusoid   SQUare   TRIangle   RAMP   NRAMp   PRNoise   ARBB   EFILe} [SOURce[n]]:FM:INTernal:FUNCTion?
<b>Related Commands</b>	[SOURce[n]]:FM:SOURce
<b>Arguments</b>	The value of n indicates the channel number. SINusoid   SQUare   TRIangle   RAMP   NRAMp   PRNoise One of six types of function waveform can be selected as a modulating signal. ARBB   EFILe can be selected as a modulating file.
<b>Returns</b>	SIN   SQU   TRI   RAMP   NRAM   PRN   ARBB   EFILe
<b>Example</b>	SOURce1:FM:INTernal:FUNCTion SQUare Select square as the shape of modulating waveform for the channel 1 (CH 1) output.

**Table 64: [SOURce[n]]:FM:INTernal:FUNCTion**

<b>Command</b>	[SOURce[n]]:FM:INTernal:FUNCTion:EFILe
<b>Description</b>	This command sets or queries the EFILe name used as a modulating waveform for FM modulation. A file name must be specified in the file system, the valid file extensions are “.txt”, “.csv” and “.trc”. If the file is not set the query returns “”. If the file contains more than 16834 samples, it will be decimated. This command returns "" if the EFILe is not set. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FM:INTernal:FUNCTion:EFILe <file_name> [SOURce[n]]:FM:INTernal:FUNCTion:EFILe?
<b>Related Commands</b>	[SOURce[n]]:FM:SOURce
<b>Arguments</b>	The value of n indicates the channel number. <file_name>::=<Qstring> specifies a file name in the file system. The path can be absolute or relative, if you insert a relative path it starts from Current Working Directory.
<b>Returns</b>	<file_name>
<b>Example</b>	SOURce1:FM:INTernal:FUNCTion:EFILe "SAMPLE1.txt" Sets a file named "SAMPLE1" in the Current Working Directory of the file system.

**Table 65: [SOURce[n]]:FM:INTernal:FUNCTion:EFILe**

<b>Command</b>	[SOURce[n]]:FM:SOURce
<b>Description</b>	This command sets or queries the source of the FM modulating signal for the specified channel. This command will cause an error if not in the frequency modulation run mode.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FM:SOURce[INTernal   EXTernal] [SOURce[n]]:FM:SOURce?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. INTernal means that the carrier waveform is modulated with the internal source. EXTernal means that the carrier waveform is modulated with an external signal.
<b>Returns</b>	INT   EXT
<b>Example</b>	SOURce1:FM:SOURce INTernal Set the channel 1 (CH 1) source of the modulating signal to internal.

**Table 66: [SOURce[n]]:FM:SOURce**

<b>Command</b>	[SOURce[n]]:FM:STATe
<b>Description</b>	This command enables or disables frequency modulation (FM). The query version of this command returns the state of frequency modulation. When you send this command and the state changes, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FM:STATe { ON   OFF   0   1 } [SOURce[n]]:FM:STATe?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. ON   1 enables FM modulation. OFF   0 disables FM modulation.
<b>Returns</b>	<NR1> 0 means disable FM modulation, 1 means enable FM modulation.
<b>Example</b>	SOURce1:FM:STATe ON Enable the channel 1 FM modulation.

**Table 67: [SOURce[n]]:FM:STATe**

<b>Command</b>	[SOURce[n]]:FREQuency[:CW   :FIXed]
----------------	-------------------------------------

<b>Description</b>	This command sets or queries the frequency of the output waveform for the specified channel. This command is available when the Run Mode is set to any setting other than Sweep. The output frequency range setting depends on the type of output waveform. If you change the type of output waveform, it may change the output frequency because changing waveform types affects the setting range of the output frequency. The output frequency range setting depends also on the amplitude parameter.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FREQUency[:CW   :FIXed] <frequency> [SOURce[n]]:FREQUency[:CW   :FIXed]? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <frequency>::=<NRf><units> Where: <NRf> is the output frequency. <units>::=[Hz   kHz   MHz] MINimum queries the minimum frequency. MAXimum queries the maximum frequency.
<b>Returns</b>	<frequency>
<b>Example</b>	SOURce1:FREQUency:FIXed 500kHz Set the channel 1 (CH 1) output frequency to 500 kHz when the Run Mode is set to any setting other than Sweep.

**Table 68: [SOURce[n]]:FREQUency[:CW | :FIXed]**

<b>Command</b>	[SOURce[n]]:FREQUency:MODE
<b>Description</b>	This command sets or queries the frequency sweep state. For the Pulse function the sweep is not allowed. When you send this command and the state changes, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FREQUency:MODE {CW   FIXed   SWEep} [SOURce[n]]:FREQUency:MODE?
<b>Related Commands</b>	[SOURce[n]]:FREQUency[:CW   :FIXed] [SOURce[n]]:FREQUency:START [SOURce[n]]:FREQUency:STOP
<b>Arguments</b>	The value of n indicates the channel number. CW   FIXed means that the instrument is in Continuous Mode. SWEep means that the instrument is in Sweep Mode.
<b>Returns</b>	CW   SWE

<b>Example</b>	SOURce1:FREQUency:MODE SWEep Specify the sweep command set for controlling the CH 1 output frequency
----------------	--

**Table 69: [SOURce[n]]:FREQUency:MODE**

<b>Command</b>	[SOURce[n]]:FREQUency:START
<b>Description</b>	This command sets or queries the start frequency of a sweep for the specified channel. This command is always used with the [SOURce[n]]:FREQUency:STOP command. The start frequency range setting depends on the waveform selected for sweep and on the amplitude in case of Sine function. This command will cause an error if not in the Sweep state. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FREQUency:START <frequency> [SOURce[n]]:FREQUency:START? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[1   2]]:FREQUency:MODE [SOURce[1   2]]:FREQUency:STOP
<b>Arguments</b>	The value of n indicates the channel number. <frequency>::=<NRf>[<units>] Where: <NRf> is the start frequency. <units>::=[Hz   kHz   MHz] MINimum queries the minimum frequency. MAXimum queries the maximum frequency.
<b>Returns</b>	<frequency>
<b>Example</b>	SOURce1:FREQUency:START 10KHz Set the start frequency of channel 1 (CH 1) to 10 kHz.

**Table 70: [SOURce[1 | 2]]:FREQUency:START**

<b>Command</b>	[SOURce[n]]:FREQUency:STOP
<b>Description</b>	This command sets or queries the stop frequency of sweep for the specified channel. This command is always used with the [SOURce[1   2]]:FREQUency:START command. The stop frequency range setting depends on the waveform selected for sweep and on the amplitude in case of Sine function. This command will cause an error if not in the Sweep state. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FREQUency:STOP <frequency> [SOURce[n]]:FREQUency:STOP? [MINimum   MAXimum]

<b>Related Commands</b>	[SOURce[n]]:FREQUency:MODE [SOURce[n]]:FREQUency:START
<b>Arguments</b>	The value of n indicates the channel number. <frequency>::=<NRf>[<units>] Where: <NRf> is the stop frequency. <units>::=[Hz   kHz   MHz]
<b>Returns</b>	<frequency>
<b>Example</b>	SOURce1:FREQUency:STOP 100kHz Set the sweep stop frequency of channel 1 (CH 1) to 100 kHz.

**Table 71: [SOURce[n]]:FREQUency:STOP**

<b>Command</b>	[SOURce[n]]:FSKey[:FREQUency]
<b>Description</b>	This command sets or queries the hop frequency of FSK modulation for the specified channel. This command will cause an error if not in the FSKEY state. When you send this command and the state changes, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FSKey[:FREQUency] <frequency> [SOURce[n]]:FSKey[:FREQUency]? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <frequency>::=<NRf>[<units>] Where: <NRf> is the hop frequency. <units>::=[Hz   kHz   MHz] MINimum queries the minimum frequency. MAXimum queries the maximum frequency.
<b>Returns</b>	<frequency>
<b>Example</b>	SOURce1:FSKey:FREQUency 1.0MHz Set the hop frequency of channel 1 FSK modulation to 1.0 MHz.

**Table 72: [SOURce[n]]:FSKey[:FREQUency]**

<b>Command</b>	[SOURce[n]]:FSKey:INTernal:RATE
<b>Description</b>	This command sets or queries the internal modulation rate of FSK modulation for the specified channel. This command will cause an error if not in the FSKEY run mode.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FSKey:INTernal:RATE <rate> [SOURce[n]]:FSKey:INTernal:RATE? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number.

	<p>&lt;rate&gt;::=&lt;NRf&gt;[&lt;units&gt;] Where: &lt;NRf&gt; is the modulation rate.          &lt;units&gt;::=[Hz   kHz   MHz]          MINimum queries the minimum delay.          MAXimum queries the maximum delay.</p>
<b>Returns</b>	<rate>
<b>Example</b>	<p>SOURce1:FSKey:INTernal:RATE 50Hz          Set the channel 1 (CH 1) internal modulation rate to 50 Hz.</p>

**Table 73: [SOURce[n]]:FSKey:INTernal:RATE**

<b>Command</b>	[SOURce[n]]:FSKey:SOURce
<b>Description</b>	This command sets or queries the source of the FSK modulation signal for the specified channel. This command will cause an error if not in the FSKEY state.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FSKey:SOURce [INTernal   EXTernal] [SOURce[n]]:FSKey:SOURce?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. INTernal means that the carrier waveform is modulated with an internal source. EXTernal means that the carrier waveform is modulated with an external signal.
<b>Returns</b>	INT   EXT
<b>Example</b>	<p>SOURce1:FSKey:SOURce INTernal          Set the channel 1 (CH 1) modulating signal source to internal.</p>

**Table 74: [SOURce[n]]:FSKey:SOURce**

<b>Command</b>	[SOURce[n]]:FSKey:STATe
<b>Description</b>	This command enables or disables FSK modulation. The query form of this command returns the state of FSK modulation. When you send this command and the state changes, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FSKey:STATe { ON   OFF   0   1 } [SOURce[n]]:FSKey:STATe?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. ON   1 enables FSK modulation. OFF   0 disables FSK modulation.



<b>Returns</b>	<NR1> 0 means OFF, 1 means ON
<b>Example</b>	SOURce1:FSKey:STATe ON Enable the channel 1 (CH 1) FSK modulation.

**Table 75: [SOURce[n]]:FSKey:STATe**

<b>Command</b>	[SOURce[n]]:PSKey[:FREQUency]
<b>Description</b>	This command sets or queries the frequency of PSK modulation for the specified channel. This command will cause an error if not in the PSK state.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PSKey[:FREQUency] <frequency> } [SOURce[n]]:PSKey[:FREQUency]? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <frequency>::=<NRf>[<units>] Where: <NRf> is the hop frequency. <units>::=[Hz   kHz   MHz]. MINimum queries the minimum frequency. MAXimum queries the maximum frequency.
<b>Returns</b>	<frequency>
<b>Example</b>	SOURce1:PSKey:FREQUency 1.0MHz Set the hop frequency of channel 1 (CH 1) PSK modulation to 1.0 MHz.

**Table 76: [SOURce[n]]:PSKey[:FREQUency]**

<b>Command</b>	[SOURce[n]]:PSKey:PHASe[:ADJust]
<b>Description</b>	This command sets or queries the phase of the modulating signal of PSKEY modulation for the specified channel. The value is in degrees. This command will cause an error if not in PSKEY run mode.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PSK:PHASe[:ADJust] <phase> } [SOURce[n]]:PSK:PHASe[:ADJust]? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <phase>::=<NR3>[<units>] Where: <NR3> is the phase of modulating signal. <units>::=[°   DEG]. MINimum queries the minimum phase value. MAXimum queries the maximum phase value.

<b>Returns</b>	<phase>
<b>Example</b>	SOURce1:PSK:PHASe:ADJust 85DEG Set the value for the phase of the channel 1 (CH 1) PSK modulating waveform to 85 degrees.

**Table 77: [SOURce[n]]:PSKey:PHASe[:ADJust]**

<b>Command</b>	[SOURce[n]]:PSKey:SOURce
<b>Description</b>	This command sets or queries the source of the PSK modulation signal for the specified channel. This command will cause an error if not in the PSKEY state.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PSKey:SOURce [INTernal   EXTernal] [SOURce[n]]:PSKey:SOURce?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. INTernal means that the carrier waveform is modulated with an internal source. EXTernal means that the carrier waveform is modulated with an external signal.
<b>Returns</b>	INT   EXT
<b>Example</b>	SOURce1:PSKey:SOURce INTernal Set the channel 1 (CH 1) source of the modulating signal to internal.

**Table 78: [SOURce[n]]:PSKey:SOURce**

<b>Command</b>	[SOURce[n]]:PSKey:STATe
<b>Description</b>	This command enables or disables PSK modulation. The query version of this command returns the state of PSK modulation. When you send this command and the state changes, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PSKey:STATe { ON   OFF   0   1 } [SOURce[n]]:PSKey:STATe?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. ON   1 enables PSK modulation. OFF   0 disables PSK modulation.
<b>Returns</b>	<NR1> 0 means OFF, 1 means ON

<b>Example</b>	SOURce1:PSKey:STATE ON Enable the channel 1 (CH 1) PSK modulation.
----------------	---

**Table 79: [SOURce[n]]:PSKey:STATE**

<b>Command</b>	[SOURce[n]]:FUNCTion:EFILe
<b>Description</b>	This command sets or queries the EFILe name used as carrier waveform. A file name must be specified in the file system, the valid file extensions are ".txt", ".csv" and ".trc". This query returns "" if the EFILe is not set. If the file contains more than 16834 samples, it will be decimated. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FUNCTion:EFILe <file_name> [SOURce[n]]:FUNCTion:EFILe?
<b>Related Commands</b>	[SOURce[n]]:FUNCTion[:SHAPe]
<b>Arguments</b>	The value of n indicates the channel number. <file_name>::= <Qstring> specifies a file name in the file system. The path can be absolute or relative, if you insert a relative path it starts from Current Working Directory.
<b>Returns</b>	<file_name>
<b>Example</b>	SOURce1:FUNCTion:EFILe "SAMPLE1.txt" Sets a file named "SAMPLE1" in the Current Working Directory of the file system.

**Table 80: [SOURce[n]]:FUNCTion:EFILe**

<b>Command</b>	[SOURce[n]]:FUNCTion:RAMP:SYMMetry
<b>Description</b>	This command sets or queries the symmetry of the ramp waveform for the specified channel. If the carrier is not "Ramp", this command causes an error.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FUNCTion:RAMP:SYMMetry <symmetry> [SOURce[n]]:FUNCTion:RAMP:SYMMetry? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <symmetry>::=<NR2>[<units>] Where: <NR2> is the symmetry. <units>::=PCT MINimum queries the minimum symmetry value. MAXimum queries the maximum symmetry value.

<b>Returns</b>	<symmetry>
<b>Example</b>	SOURce1:FUNCTION:RAMP:SYMMetry 80.5 Set the symmetry of the channel 1 (CH 1) ramp waveform to 80.5%

**Table 81: [SOURce[n]]:FUNCTION:RAMP:SYMMetry**

<b>Command</b>	[SOURce[n]]:FUNCTION[:SHAPE]
<b>Description</b>	This command sets or queries the shape of the carrier waveform. Setting the carrier, it is necessary to meet some condition listed in the below table. When you send this command and the function changes, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:FUNCTION[:SHAPE] {SINusoid   SQUare   PULSe   RAMP   PRNoise   DC   SINC   GAUSSian   LORentz   ERISe   EDECay   HAVersine   ARBB   EFILe   DOUBLEPULse} [SOURce[n]]:FUNCTION[:SHAPE]?
<b>Related Commands</b>	None
<b>Arguments</b>	<p>The value of n indicates the channel number. SINusoid   SQUare   PULSe   RAMP   PRNoise   DC   SINC   GAUSSian   LORentz   ERISe   EDECay   HAVersine   ARBB   EFILe   DOUBLEPULse</p> <p>If you select a waveform shape that is not allowed with a particular modulation, sweep, or burst, it causes an error and the function does not change. If you specify EFILe when there is no EFILe or the EFILe is not yet defined, this command causes an error and the change will not be applied. If you change the waveform, the output frequency may change to meet the frequency range of the new waveform. If you select "PRNoise" when the additive noise is on, it causes an error. To disable the additive noise use the command: [SOURce[n]]:COMBine:FEED. When you send this command, if the instrument is running it will be stopped.</p> <p>The following table shows the combinations of modulation type and the shape of output waveform.</p>

	Sine, Square, Ramp, Sinc, Gaussian, Lorentz, Exponential Rise, Exponential Decay, Haversine, ARBB, EFILE	Pulse	Double Pulse	Noise, DC																																																												
AM	✓																																																															
FM	✓																																																															
PM	✓																																																															
FSK	✓																																																															
PSK	✓																																																															
PWM		✓																																																														
Sweep	✓																																																															
Burst	✓	✓	✓																																																													
<p>The following table shows the combinations of voltage unit for the amplitude and the shape of output waveform.</p> <table border="1"> <thead> <tr> <th></th> <th>Vpp</th> <th>Vrms</th> <th>dBm</th> </tr> </thead> <tbody> <tr> <td>Sine</td> <td>✓</td> <td>✓</td> <td>✓</td> </tr> <tr> <td>Square</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Ramp</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Pulse</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Sinc</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Noise</td> <td>✓ (Vpk)</td> <td></td> <td></td> </tr> <tr> <td>DC level</td> <td></td> <td></td> <td></td> </tr> <tr> <td>Gaussian</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Lorentz</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Exponential Rise</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Exponential Decay</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Haversine</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>ARBB</td> <td>✓</td> <td></td> <td></td> </tr> <tr> <td>EFILE</td> <td>✓</td> <td></td> <td></td> </tr> </tbody> </table>						Vpp	Vrms	dBm	Sine	✓	✓	✓	Square	✓	✓		Ramp	✓	✓		Pulse	✓	✓		Sinc	✓	✓		Noise	✓ (Vpk)			DC level				Gaussian	✓	✓		Lorentz	✓	✓		Exponential Rise	✓	✓		Exponential Decay	✓	✓		Haversine	✓	✓		ARBB	✓			EFILE	✓		
	Vpp	Vrms	dBm																																																													
Sine	✓	✓	✓																																																													
Square	✓	✓																																																														
Ramp	✓	✓																																																														
Pulse	✓	✓																																																														
Sinc	✓	✓																																																														
Noise	✓ (Vpk)																																																															
DC level																																																																
Gaussian	✓	✓																																																														
Lorentz	✓	✓																																																														
Exponential Rise	✓	✓																																																														
Exponential Decay	✓	✓																																																														
Haversine	✓	✓																																																														
ARBB	✓																																																															
EFILE	✓																																																															
<b>Returns</b>	SIN   SQU   PULS   RAMP   PRN   DC   SINC   GAUS   LOR   ERIS   EDEC   HAV   ARBB   EFILE   DOUBLEPULSe																																																															
<b>Example</b>	SOURce1:FUNCTION:SHAPE SQUARE Select the shape of channel 1 output waveform to square waveform.																																																															

**Table 82: [SOURCE[n]]:FUNCTION[:SHAPE]**

<b>Command</b>	[SOURce[n]]:INITDElay
<b>Description</b>	This command sets or queries the initial delay for the selected output channel. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:INITDElay <delay> [SOURce[n]]:INITDElay? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <delay>::=<NRf>[<units>] Where: <NRf> is the initial delay value. <units>::=[ns   μs   ms   s] MINimum queries the minimum delay. MAXimum queries the maximum delay.
<b>Returns</b>	<delay>
<b>Example</b>	SOURce1:INITDElay 300E-9 Set the output 1 initial delay to 300 ns.

**Table 83: [SOURce[n]]:INITDElay**

<b>Command</b>	[SOURce[n]]:PHASe[:ADJust]
<b>Description</b>	This command sets or queries the phase of the output waveform for the specified channel. The value is in degrees.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PHASe[:ADJust] <phase> [SOURce[n]]:PHASe[:ADJust]? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <phase>::=<NR3>[<units>] Where: <NR3> is the phase of output frequency. <units>::=[°   DEG]. MINimum queries the minimum phase value. MAXimum queries the maximum phase value.
<b>Returns</b>	<phase>

<b>Example</b>	SOURce1:PHASe 45DEG Set the phase to 45 degrees
----------------	--

**Table 84: [SOURce[n]]:PHASe[:ADJust]**

<b>Command</b>	[SOURce[n]]:PM[:DEViation]
<b>Description</b>	This command sets or queries the peak frequency deviation of PM modulation for the specified channel. This command will cause an error if not in PM mode.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PM:DEViation <deviation> [SOURce[n]]:PM:DEViation? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <deviation>::=<NR3>[<units>] Where: <NR3> is the phase deviation. <units>::=[°   DEG]. MINimum queries the minimum deviation. MAXimum queries the maximum deviation.
<b>Returns</b>	<deviation>
<b>Example</b>	SOURce1:PM:DEViation 60 DEG Set the phase deviation for the channel 1 to 60 degrees.

**Table 85: [SOURce[n]]:PM[:DEViation]**

<b>Command</b>	[SOURce[n]]:PM:INTernal:FREQuency
<b>Description</b>	This command sets or queries the internal modulation frequency of PM modulation for the specified channel. You can use this command only when the internal modulation source is selected. This command will cause an error if not in PM mode.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PM:INTernal:FREQuency <frequency> [SOURce[n]]:PM:INTernal:FREQuency? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:PM:SOURce
<b>Arguments</b>	The value of n indicates the channel number. <frequency>::=<NRf>[<units>] Where: <NRf> is the modulation frequency. <units>::=[Hz   kHz   MHz] MINimum queries the minimum frequency. MAXimum queries the maximum frequency.
<b>Returns</b>	<frequency>

<b>Example</b>	SOURce1:PM:INTernal:FREQUency 10kHz Set the channel 1 (CH 1) internal modulation frequency to 10 kHz
----------------	---

**Table 86: [SOURce[n]]:PM:INTernal:FREQUency**

<b>Command</b>	[SOURce[n]]:PM:INTernal:FUNcTion
<b>Description</b>	This command sets or queries the modulating waveform of PM modulation for the specified channel. You can use this command only when the internal modulation source is selected. If you specify EFILE when there is no EFILE or the EFILE is not yet defined, this command causes an error. This command will cause an error if not in PM mode. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PM:INTernal:FUNcTion {SINusoid   SQUare   TRIangle   RAMP   NRAMp   PRNoise   ARBB   EFILE} [SOURce[n]]:PM:INTernal:FUNcTion?
<b>Related Commands</b>	[SOURce[n]]:PM:SOURce
<b>Arguments</b>	The value of n indicates the channel number. SINusoid   SQUare   TRIangle   RAMP   NRAMp   PRNoise One of six types of function waveform can be selected as a modulating function. ARBB   EFILE can be selected as a modulating file.
<b>Returns</b>	SIN   SQU   TRI   RAMP   NRAM   PRN   ARBB   EFILE
<b>Example</b>	SOURce1:PM:INTernal:FUNcTion SQUare Select square as the shape of modulating waveform for the channel 1 (CH 1) output.

**Table 87: [SOURce[n]]:PM:INTernal:FUNcTion**

<b>Command</b>	[SOURce[n]]:PM:INTernal:FUNcTion:EFILE
<b>Description</b>	This command sets or queries an EFILE name used as a modulating waveform for PM modulation. A file name must be specified in the file system, the valid file extensions are ".txt", ".csv" and ".trc". This query returns "" if the EFILE is not set. If the file contains more than 16834 samples, it will be decimated. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PM:INTernal:FUNcTion:EFILE <file_name> [SOURce[n]]:PM:INTernal:FUNcTion:EFILE?
<b>Related Commands</b>	[SOURce[n]]:PM:SOURce



<b>Arguments</b>	The value of n indicates the channel number. <file_name>::=<Qstring> specifies a file name in the file system. The <file_name> includes the path. The path can be absolute or relative, if you insert a relative path it starts from Current Working Directory.
<b>Returns</b>	<file_name>
<b>Example</b>	SOURce1:PM:INTernal:FUNCTion:EFILe "SAMPLE1.txt" Sets up a file named "SAMPLE1" in the Current Working Directory of the file system.

**Table 88: [SOURce[n]]:PM:INTernal:FUNCTion:EFILe**

<b>Command</b>	[SOURce[n]]:PM:SOURce
<b>Description</b>	This command sets or queries the source of the PM modulation signal for the specified channel. This command will cause an error if not in PM mode.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PM:SOURce [INTernal   EXTernal] [SOURce[n]]:PM:SOURce?
<b>Related Commands</b>	[SOURce[n]]:PM:SOURce
<b>Arguments</b>	The value of n indicates the channel number. INTernal means that the carrier waveform is modulated with an internal source. EXTernal means that the carrier waveform is modulated with an external signal.
<b>Returns</b>	INT   EXT
<b>Example</b>	SOURce1:PM:SOURce INTernal Set the channel 1 (CH 1) source of the modulating signal to internal.

**Table 89: [SOURce[n]]:PM:SOURce**

<b>Command</b>	[SOURce[n]]:PM:STATe
<b>Description</b>	This command enables or disables PM modulation. The query version of this command returns the state of PM modulation. When you send this command and the state changes, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PM:STATe {ON   OFF   0   1} [SOURce[n]]:PM:STATe?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number.

	ON   1 enables PM modulation. OFF   0 disables PM modulation.
<b>Returns</b>	<NR1> 0 means OFF, 1 means ON
<b>Example</b>	SOURce1:PM:STATe ON Enable the channel 1 (CH 1) PM modulation

**Table 90: [SOURce[n]]:PM:STATe**

<b>Command</b>	[SOURce[n]]:POWER[:LEVel][:IMMediate][:AMPLitude]
<b>Description</b>	This command sets or queries the internal noise level to add to the output signal for the specified channel. The value represents the peak voltage of the noise level. You can set or query whether to add the internal noise to the output signal using the [SOURce[n]]:COMBine:FEED command.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:POWER[:LEVel][:IMMediate][:AMPLitude] {<voltage>   MINimum   MAXimum} [SOURce[n]]:POWER[:LEVel][:IMMediate][:AMPLitude]? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COMBine:FEED
<b>Arguments</b>	The value of n indicates the channel number. <voltage>::=<NR3><units> Where: <NR3> is the peak noise level. <units>::=[mV   V] MINimum sets or queries the minimum noise level. MAXimum sets or queries the maximum noise level.
<b>Returns</b>	<voltage>
<b>Example</b>	SOURce1:POWER:LEVel:IMMediate:AMPLitude 0.5 Set the internal noise level that is added to the CH1 output signal to 0.5 Vpk.

**Table 91: [SOURce[n]]:POWER[:LEVel][:IMMediate][:AMPLitude]**

<b>Command</b>	[SOURce[n]]:PULSe:DCYClE
<b>Description</b>	This command sets or queries the duty cycle of the pulse waveform for the specified channel. The arbitrary function generator will hold the settings of leading edge and trailing edge when the duty cycle

	is varied. If the carrier is different from Pulse, this command and this query cause an error.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PULSe:DCYCLE <percent> [SOURce[n]]:PULSe:DCYCLE? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:PULSe:WIDTh
<b>Arguments</b>	The value of n indicates the channel number. <percent>::=<NR2>[<units>] Where: <NR2> is the duty cycle. <units>::=PCT MINimum queries the minimum duty cycle. MAXimum queries the maximum duty cycle.
<b>Returns</b>	<percent>
<b>Example</b>	SOURce1:PULSe:DCYCLE 80.5 Set the duty cycle of the pulse waveform on channel 1 (CH 1) to 80.5%.

**Table 92: [SOURce[n]]:PULSe:DCYCLE**

<b>Command</b>	[SOURce[n]]:PULSe:PERiod
<b>Description</b>	This command sets or queries the period for the pulse waveform. This command and this query will cause an error if the carrier function is different from Pulse. NOTE: the pulse period is related to the frequency, then if you change the pulse period, it also affects the frequency of the next carrier that you set.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PULSe:PERiod <period> [SOURce[n]]:PULSe:PERiod? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <period>::=<NRf>[<units>] Where: <NRf> is the pulse period. <units>::=[ns   μs   ms   s] MINimum queries the minimum period. MAXimum queries the maximum period.
<b>Returns</b>	<period>
<b>Example</b>	SOURce1:PULSe:PERiod 200ns Set the channel 1 pulse period to 200 ns.

**Table 92: [SOURce[n]]:PULSe:PERiod**

<b>Command</b>	[SOURce[n]]:PULSe:TRANSition[:LEADing]
----------------	--

<b>Description</b>	This command sets or queries the leading edge time of the pulse waveform. Note that the value is about the leading edge between 10% and 90%. If the carrier is different from Pulse, this command and this query cause an error.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PULSe:TRANSition[:LEADing] <seconds> [SOURce[n]]:PULSe:TRANSition[:LEADing]? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:PULSe:TRANSition:TRAILing
<b>Arguments</b>	The value of n indicates the channel number. <seconds>::=<NRf><units> Where: <NRf> is the leading edge time of pulse waveform. <units>::=[ns   μs   ms   s] MINimum queries the minimum transition time. MAXimum queries the maximum transition time.
<b>Returns</b>	<seconds>
<b>Example</b>	SOURce1:PULSe:TRANSition:LEADing 200ns Set the channel 1 (CH 1) leading edge time to 200 ns

**Table 93: [SOURce[n]]:PULSe:TRANSition[:LEADing]**

<b>Command</b>	[SOURce[n]]:PULSe:TRANSition:TRAILing
<b>Description</b>	This command sets or queries the trailing edge time of the pulse waveform. Note that the value is about the leading edge between 10% and 90%. If the carrier is different from Pulse, this command and this query cause an error.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PULSe:TRANSition:TRAILing <seconds> [SOURce[n]]:PULSe:TRANSition:TRAILing? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:PULSe:TRANSition[:LEADing]
<b>Arguments</b>	The value of n indicates the channel number. <seconds>::=<NRf><units>. Where: <NRf> is the trailing edge of pulse waveform. <units>::=[ns   μs   ms   s] MINimum queries the minimum delay. MAXimum queries the maximum delay.
<b>Returns</b>	<seconds>
<b>Example</b>	SOURce1:PULSe:TRANSition:TRAILing 200ns Set the trailing edge time to 200 ns.

**Table 94: [SOURce[n]]:PULSe:TRANSition:TRAILing**

<b>Command</b>	[SOURce[n]]:PULSe:WIDTH
----------------	-------------------------

<b>Description</b>	This command sets or queries the pulse width for the specified channel. Pulse Width = Period × Duty Cycle / 100. The pulse width must be less than the period. If the carrier is different from Pulse, this command and this query cause an error.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PULSe:WIDTh <seconds> [SOURce[n]]:PULSe:WIDTh? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:PULSe:DCYCLE
<b>Arguments</b>	The value of n indicates the channel number. <seconds>::=<NRf>[<units>] Where: <NRf> is the pulse width. <units>::=[ns   μs   ms   s] MINimum queries the minimum delay. MAXimum queries the maximum delay.
<b>Returns</b>	<width>
<b>Example</b>	SOURce1:PULSe:WIDTh 200ns Set the channel 1 (CH 1) pulse width to 200 ns.

**Table 95: [SOURce[n]]:PULSe:WIDTh**

<b>Command</b>	[SOURce[n]]:PWM:INTernal:FREQuency
<b>Description</b>	This command sets or queries the internal modulation frequency of PWM modulation for the specified channel. You can use this command only when the internal modulation source is selected. This command will cause an error if not in PWM mode.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PWM:INTernal:FREQuency <frequency> [SOURce[n]]:PWM:INTernal:FREQuency? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:PWM:SOURce
<b>Arguments</b>	The value of n indicates the channel number. <frequency>::=<NRf>[<units>] Where: <NRf> is the modulation frequency. <units>::=[Hz   kHz   MHz] MINimum queries the minimum frequency. MAXimum queries the maximum frequency.
<b>Returns</b>	<frequency>
<b>Example</b>	SOURce1:PWM:INTernal:FREQuency 10kHz Set the channel 1 (CH 1) internal frequency to 10 kHz.

**Table 96: [SOURce[n]]:PWM:INTernal:FREQuency**

<b>Command</b>	[SOURce[n]]:PWM:INTernal:FUNctIon
<b>Description</b>	This command sets or queries the modulating waveform of PWM modulation for the specified channel. You can use this command only when the internal modulation source is selected. If you specify EFILE when there is no EFILE or the EFILE is not yet defined, this command causes an error. This command will cause an error if not in PWM mode. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PWM:INTernal:FUNctIon {SINusoid   SQUare   TRIangle   RAMP   NRAMp   PRNoise   ARBB   EFILE} [SOURce[n]]:PWM:INTernal:FUNctIon?
<b>Related Commands</b>	[SOURce[n]]:PWM:SOURce
<b>Arguments</b>	The value of n indicates the channel number. SINusoid   SQUare   TRIangle   RAMP   NRAMp   PRNoise One of six types of function waveform can be selected as a modulating signal. ARBB   EFILE can be selected as a modulating file.
<b>Returns</b>	SIN   SQU   TRI   RAMP   NRAM   PRN   ARBB   EFILE
<b>Example</b>	SOURce1:PWM:INTernal:FUNctIon SQUare Select square as the shape of modulating waveform for the channel 1 output.

**Table 97: [SOURce[n]]:PWM:INTernal:FUNctIon**

<b>Command</b>	[SOURce[n]]:PWM:INTernal:FUNctIon:EFILE
<b>Description</b>	This command sets or queries an EFILE name used as a modulating waveform for PWM modulation. A file name must be specified in the file system, the valid file extensions are ".txt", ".csv" and ".trc". The query version of this command returns "" if the the EFILE is not set. If the file contains more than 16834 samples, it will be decimated. When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PWM:INTernal:FUNctIon:EFILE <file_name> [SOURce[n]]:PWM:INTernal:FUNctIon:EFILE?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number.

	<file_name>::=<Qstring> specifies a file name in the file system. The <file_name> parameter includes the path. The path can be absolute or relative, if you insert a relative path it starts from Current Working Directory.
<b>Returns</b>	<file_name>
<b>Example</b>	SOURce1:PWM:INTernal:FUNction:EFILe "SAMPLE1.txt" Sets a file named "SAMPLE1" in the Current Working Directory of the file system.

**Table 98: [SOURce[n]]:PWM:INTernal:FUNction:EFILe**

<b>Command</b>	[SOURce[n]]:PWM:SOURce
<b>Description</b>	This command sets or queries the source of the modulating signal of PWM modulation for the specified channel. This command will cause an error if not in PWM run mode.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PWM:SOURce[INTernal   EXTernal] [SOURce[n]]:PWM:SOURce?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. INTernal means that the carrier waveform is modulated with the internal source. EXTernal means that the carrier waveform is modulated with an external signal.
<b>Returns</b>	INT   EXT
<b>Example</b>	SOURce1:PWM:SOURce INTernal Set the source of the modulating signal on channel 1 to internal.

**Table 99: [SOURce[n]]:PWM:SOURce**

<b>Command</b>	[SOURce[n]]:PWM:STATe
<b>Description</b>	This command enables or disables PWM modulation. The query form of this command returns the state of PWM modulation. Before activate the PWM it is necessary to select the Pulse as carrier.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PWM:STATe {ON   OFF   0   1} [SOURce[n]]:PWM:STATe?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. ON   1 enables PWM modulation.

	OFF   0 disables PWM modulation.
<b>Returns</b>	<NR1> 0 means OFF, 1 means ON
<b>Example</b>	SOURce1:PWM:STATE ON Enable the channel 1 PWM modulation.

**Table 100: [SOURce[n]]:PWM:STATE**

<b>Command</b>	[SOURce[n]]:PWM[:DEVIation]:DCYCLE
<b>Description</b>	This command sets or queries the PWM deviation in percent for the specified channel. The setting range must meet the following conditions: <input type="checkbox"/> Deviation $\leq$ Pulse Width – PWmin <input type="checkbox"/> Deviation $\leq$ Pulse Period – Pulse Width – PWmin <input type="checkbox"/> Deviation $\leq$ Pulse Width – (Leading Edge Time + Trailing Edge Time) /0.8 <input type="checkbox"/> Deviation $\leq$ Pulse Period – Pulse Width – (Leading Edge Time + Trailing Edge Time) /0.8 <input type="checkbox"/> Where: PWmin is the minimum pulse width. This command will cause an error if not in PWM mode.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:PWM[:DEVIation]:DCYCLE <percent> [SOURce[n]]:PWM[:DEVIation]:DCYCLE? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <percent>::=<NR2>[<units>] Where: <NR2> is the PWM deviation. <units>::=PCT
<b>Returns</b>	<deviation>
<b>Example</b>	SOURce1:PWM:DCYCLE 5.0 Set the channel 1 (CH 1) PWM deviation to 5.0%

**Table 101: [SOURce[n]]:PWM[:DEVIation]:DCYCLE**

<b>Command</b>	[SOURce]:ROSCillator:FREQUENCY
<b>Description</b>	This command sets or queries the clock frequency of the external reference.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce]:ROSCillator:FREQUENCY <frequency> [SOURce]:ROSCillator:FREQUENCY? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce]:ROSCillator:SOURce



<b>Arguments</b>	The value of n indicates the channel number. <frequency>::=<NRf>[<units>] Where: <NRf> is the external reference frequency. <units>::=[Hz   kHz   MHz] MINimum queries the minimum frequency. MAXimum queries the maximum frequency.
<b>Returns</b>	<frequency>
<b>Example</b>	SOURce:ROSCillator:FREQUENCY 10MHZ Set the reference clock in to 10 MHz.

**Table 102: [SOURce]:ROSCillator:FREQUENCY**

<b>Command</b>	[SOURce]:ROSCillator:SOURce
<b>Description</b>	This command sets or queries the reference clock to either internal or external. When you try to set External, if the frequency of the external reference is different from the frequency set through [SOURce]:ROSCillator:FREQUENCY command, this command causes an error and the source will be reset to Internal.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce]:ROSCillator:SOURce {INTernal   EXTernal} [SOURce]:ROSCillator:SOURce?
<b>Related Commands</b>	[SOURce]:ROSCillator:FREQUENCY
<b>Arguments</b>	The value of n indicates the channel number. INTernal means that the reference clock is set to internal. EXTernal means that the reference clock is set to external.
<b>Returns</b>	INT   EXT
<b>Example</b>	SOURce:ROSCillator:SOURce INTernal Select the internal clock reference.

**Table 103: [SOURce]:ROSCillator:SOURce**

<b>Command</b>	[SOURce[n]]:SWEep:NSTEP
<b>Description</b>	This command sets or queries the Number of Step of the Upstair Sweep. The step number ranges from 1 to 2,048. This command will cause an error if not in Upstair Sweep mode.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:SWEep:NSTEP <step number> [SOURce[n]]:SWEep:NSTEP? [MINimum   MAXimum]
<b>Related Commands</b>	None

<b>Arguments</b>	The value of n indicates the channel number. <step number>::=<NR1> Where: <NR1> is the burst count. MINimum queries the minimum number of steps. MAXimum queries the maximum number of steps.
<b>Returns</b>	<step number>
<b>Example</b>	SOURce1:SWEEp:NSTEP 8 Sets the channel 1 sweep step to 8.

**Table 104: [SOURce[n]]:SWEEp:NSTEP**

<b>Command</b>	[SOURce[n]]:SWEEp:HTIME
<b>Description</b>	This command sets or queries the sweep hold time. Hold time represents the amount of time that the frequency remains stable after reaching the stop frequency. This command and this query will cause an error if not in Sweep mode. Is not possible modify the hold time while the instrument is running, if this command is sent during the running mode an error occurs.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:SWEEp:HTIME <seconds> [SOURce[n]]:SWEEp:HTIME? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <seconds>::=<NRf><units> Where: <NRf> is the hold time in seconds. <units>::=[ns   μs   ms   s] MINimum queries the minimum hold time. MAXimum queries the maximum hold time.
<b>Returns</b>	<seconds>
<b>Example</b>	SOURce1:SWEEp:HTIME 1ms Sets the channel 1 hold time to 1 ms.

**Table 105: [SOURce[n]]:SWEEp:HTIME**

<b>Command</b>	[SOURce[n]]:SWEEp:MODE
<b>Description</b>	This command selects repeat or trigger for the sweep trigger mode for the specified channel. The query version of this command returns the sweep trigger mode for the specified channel.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:SWEEp:MODE {AUTO   MANUal} [SOURce[n]]:SWEEp:MODE?
<b>Related Commands</b>	None

<b>Arguments</b>	The value of n indicates the channel number. AUTO sets the sweep mode to repeat generation. The instrument outputs a continuous sweep at a rate specified by Sweep Rise Time, Hold Time, and Return Time. MANual sets the sweep mode to trigger. The instrument outputs one sweep when a trigger input is received and wait on the start frequency.
<b>Returns</b>	AUTO   MAN
<b>Example</b>	SOURce1:SWEEp:MODE AUTO Set the channel 1 sweep mode to repeat. The instrument outputs a continuous sweep.

**Table 106: [SOURce[n]]:SWEEp:MODE**

<b>Command</b>	[SOURce[n]]:SWEEp:RTIME
<b>Description</b>	This command sets or queries the sweep return time. Return time represents the amount of time from stop frequency through start frequency. Return time does not include hold time. This command and this query will cause an error if not in Sweep mode. Is not possible modify the return time while the instrument is running, if this command is sent during the running mode an error occurs.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:SWEEp:RTIME <seconds> [SOURce[n]]:SWEEp:RTIME? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <seconds>::=<NRf>[<units>] Where: <NRf> is the return time in seconds. <units>::=[ns   μs   ms   s] MINimum queries the minimum return time. MAXimum queries the maximum return time.
<b>Returns</b>	<return time>
<b>Example</b>	SOURce1:SWEEp:RTIME 1ms Sets the channel 1 (CH 1) return time to 1 ms.

**Table 107: [SOURce[n]]:SWEEp:RTIME**

<b>Command</b>	[SOURce[n]]:SWEEp:SPACing
<b>Description</b>	This command selects the spacing for the sweep for the specified channel. The query form of this command returns the type for the

	sweep spacing for the specified channel. When you send this command, if the instrument is running it will be stopped. NOTE: when you select USER or ARBB the time to walk the sweep profile is given by the sum of sweep rise time, sweep hold time and sweep return time.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:SWEep:SPACing {LINear   LOGarithmic   UPStair   ARBB   USER} [SOURce[n]]:SWEep:SPACing?
<b>Related Commands</b>	[SOURce[n]]:SWEep:NSTEP [SOURce[n]]:SWEep:SPACing:EFILe
<b>Arguments</b>	The value of n indicates the channel number. LINear sets the sweep spacing to linear. LOGarithmic sets the sweep spacing to logarithmic. UPStair sets the sweep spacing to stepped. ARBB allows to import a sweep profile from the arbitrary buffer. USER allows to import a sweep profile from EFILE.
<b>Returns</b>	LIN   LOG   UPS   USER   ARBB
<b>Example</b>	SOURce1:SWEep:SPACing LINear Set the channel 1 (CH1) sweep spacing to linear.

**Table 108: [SOURce[n]]:SWEep:SPACing**

<b>Command</b>	[SOURce[n]]:SWEep:SPACing:EFILe
<b>Description</b>	This command sets or queries an EFILE name used as sweep profile. A file name must be specified in the file system, the valid file extensions are ".txt", ".csv" and ".trc". If the file is not set the query returns "". If the file contains more than 16834 samples, it will be decimated. The query version of this command returns "" if the the EFILE is not set.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:SWEep:SPACing:EFILe <file_name> [SOURce[n]]:SWEep:SPACing:EFILe?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <file_name>::=<Qstring> specifies a file name in the file system. The <file_name> parameter includes the path. The path can be absolute or relative, if you insert a relative path it starts from Current Working Directory.

<b>Returns</b>	<file_name>
<b>Example</b>	SOURce1:SWEEp:SPACing:EFILe "SAMPLE1.txt" Sets a file named "SAMPLE1" in the Current Working Directory of the file system.

**Table 109: [SOURce[n]]:SWEEp:SPACing:EFILe**

<b>Command</b>	[SOURce[n]]:SWEEp:TIME
<b>Description</b>	This command sets or queries the sweep rise time for the sweep. The sweep time does not include hold time and return time. This command will cause an error if not in Sweep mode. Is not possible modify the rise time while the instrument is running, if this command is sent during the running mode an error occurs.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:SWEEp:TIME <seconds> [SOURce[n]]:SWEEp:TIME? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <seconds>::=<NRf>[<units>] Where: <NRf> is the sweep rise time in seconds. <units>::=[ns   $\mu$ s   ms   s] MINimum queries the minimum sweep rise time. MAXimum queries the maximum sweep rise time.
<b>Returns</b>	<sweep time>
<b>Example</b>	SOURce1:SWEEp:TIME 100ms Set the channel 1 (CH 1) sweep rise time to 100 ms.

**Table 110: [SOURce[n]]:SWEEp:TIME**

<b>Command</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:HIGH
<b>Description</b>	This command sets or queries the high level of the waveform for the specified channel. The high level could be limited by noise level to not exceed the maximum amplitude. If the carrier is Noise or DC level, this command and this query cause an error.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:HIGH <voltage> [SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:HIGH? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:LOW
<b>Arguments</b>	The value of n indicates the channel number.

	<voltage>::=<NRf><units>] Where: <NRf> is the high level of output amplitude. <units>::=[mV   V] MINimum queries the minimum high voltage level. MAXimum queries the maximum high voltage level.
<b>Returns</b>	<high level>
<b>Example</b>	SOURce1:VOLTage:LEVel:IMMEDIATE:HIGH 1V Set the high level of channel 1 (CH 1) output amplitude to 1 V.

**Table 111: [SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:HIGH**

<b>Command</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:LOW
<b>Description</b>	This command sets or queries the low level of the waveform for the specified channel. The low level could be limited by noise level to not exceed the maximum amplitude. If the carrier is Noise or DC level, this command and this query cause an error.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:LOW <voltage> } [SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:LOW? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:HIGH
<b>Arguments</b>	The value of n indicates the channel number. <voltage>::=<NRf><units>] Where: <NRf> is the low level of the output amplitude. <units>::=[mV   V] MINimum queries the minimum low voltage level. MAXimum queries the maximum low voltage level.
<b>Returns</b>	<low level>
<b>Example</b>	SOURce1:VOLTage:LEVel:IMMEDIATE:LOW -1V Set the low level of channel 1 (CH 1) output amplitude to -1 V.

**Table 112: [SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:LOW**

<b>Command</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:OFFSet
<b>Description</b>	This command sets or queries the offset level for the specified channel. The offset range setting depends on the amplitude parameter.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:OFFSet <voltage> [SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:OFFSet? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE][:AMPLitude]

<b>Arguments</b>	The value of n indicates the channel number. <voltage>::=<NRf>[<units>] Where: <NRf> is the offset voltage level. <units>::=[mV   V] MINimum queries the minimum offset level. MAXimum queries the maximum offset level.
<b>Returns</b>	<offset>
<b>Example</b>	SOURce1:VOLTage:LEVel:IMMEDIATE:OFFSet 500mV Set the channel 1 offset level to 500 mV.

**Table 113: [SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:OFFSet**

<b>Command</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE][:AMPLitude]
<b>Description</b>	This command sets or queries the output amplitude for the specified channel. The measurement unit of amplitude depends on the selection operated using the [SOURce[n]]:VOLTage:UNIT command. If the carrier is Noise the amplitude is Vpk instead of Vpp. If the carrier is DC level this command causes an error. The range of the amplitude setting could be limited by the frequency and offset parameter of the carrier waveform.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE][:AMPLitude] <amplitude> [SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE][:AMPLitude]? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE]:OFFSet [SOURce[n]]:VOLTage:UNIT
<b>Arguments</b>	The value of n indicates the channel number. <amplitude>::=<NRf> Where: <NRf> is the output amplitude. This parameter does not have the measurement unit because it is defined by [SOURce[n]]:VOLTage:UNIT command. MINimum queries the minimum amplitude. MAXimum queries the maximum amplitude.
<b>Returns</b>	<amplitude><unit> Where <units>::=[VPP   VRMS   DBM   VPK] VPK is used only for the noise as carrier.
<b>Example</b>	SOURce1:VOLTage:LEVel:IMMEDIATE:AMPLitude 1 Set the channel 1 output amplitude to 1, the unit depends on the selecting one.

**Table 114: [SOURce[n]]:VOLTage[:LEVel][:IMMEDIATE][:AMPLitude]**

<b>Command</b>	[SOURce[n]]:VOLTage:UNIT																																																												
<b>Description</b>	This command sets or queries the units of output amplitude for the specified channel. This command does not affect the offset, high level, or low level of output.																																																												
<b>Group</b>	Source																																																												
<b>Syntax</b>	[SOURce[n]]:VOLTage:UNIT [VPP   VRMS   DBM] [SOURce[n]]:VOLTage:UNIT?																																																												
<b>Related Commands</b>	[SOURce[n]]:VOLTage[:LEVel][:IMMediate][:AMPLitude]																																																												
<b>Arguments</b>	<p>The value of n indicates the channel number.  VPP sets the units of the output voltage to Vp-p.  VRMS sets the units of the output voltage to Vrms.  DBM sets the units of the output voltage to dBm.</p> <p>The following table shows the possible association between waveform and measurement unit for the amplitude.</p> <table border="1"> <thead> <tr> <th></th> <th>Vpp</th> <th>Vrms</th> <th>dBm</th> </tr> </thead> <tbody> <tr> <td>Sine</td> <td>✓</td> <td>✓</td> <td>✓</td> </tr> <tr> <td>Square</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Ramp</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Pulse</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Sinc</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Noise</td> <td>✓ (Vpk)</td> <td></td> <td></td> </tr> <tr> <td>DC level</td> <td></td> <td></td> <td></td> </tr> <tr> <td>Gaussian</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Lorentz</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Exponential Rise</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Exponential Decay</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>Haversine</td> <td>✓</td> <td>✓</td> <td></td> </tr> <tr> <td>ARBB</td> <td>✓</td> <td></td> <td></td> </tr> <tr> <td>EFILE</td> <td>✓</td> <td></td> <td></td> </tr> </tbody> </table>		Vpp	Vrms	dBm	Sine	✓	✓	✓	Square	✓	✓		Ramp	✓	✓		Pulse	✓	✓		Sinc	✓	✓		Noise	✓ (Vpk)			DC level				Gaussian	✓	✓		Lorentz	✓	✓		Exponential Rise	✓	✓		Exponential Decay	✓	✓		Haversine	✓	✓		ARBB	✓			EFILE	✓		
	Vpp	Vrms	dBm																																																										
Sine	✓	✓	✓																																																										
Square	✓	✓																																																											
Ramp	✓	✓																																																											
Pulse	✓	✓																																																											
Sinc	✓	✓																																																											
Noise	✓ (Vpk)																																																												
DC level																																																													
Gaussian	✓	✓																																																											
Lorentz	✓	✓																																																											
Exponential Rise	✓	✓																																																											
Exponential Decay	✓	✓																																																											
Haversine	✓	✓																																																											
ARBB	✓																																																												
EFILE	✓																																																												
<b>Returns</b>	VPP   VRMS   DBM																																																												
<b>Example</b>	SOURce1:VOLTage:UNIT VPP Set the voltage units to Vp-p.																																																												

**Table 115: [SOURce[n]]:VOLTage:UNIT**

<b>Command</b>	[SOURce[n]]:VOLTage:VOCM
----------------	--------------------------



<b>Description</b>	This command sets or queries the DC Common Mode Offset for the specified channel. The Common refers to 0V.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:VOLTage:VOCM <voltage> [SOURce[n]]:VOLTage:VOCM? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. <voltage>::=<NRf>[<units>] Where: <NRf> is the DC Offset value. <units>::=[mV   V] MINimum queries the minimum common voltage. MAXimum queries the maximum common voltage.
<b>Returns</b>	<voltage>
<b>Example</b>	SOURce1:VOLTage:VOCM 2V Set the DC common mode offset of channel 1 output to 2 V.

**Table 116: [SOURce[n]]:VOLTage:VOCM**

<b>Command</b>	[SOURce[n]]:DOUBLEPULSe:PULSe[m]:AMPLitude
<b>Description</b>	This command sets or queries the amplitude of the first or of the second pulse for the specified channel in the double pulse waveform.  Note: If the carrier is different from Double Pulse, this command and this query cause an error.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:DOUBLEPULSe:PULSe[m]:AMPLitude [SOURce[n]]:DOUBLEPULSe:PULSe[m]:AMPLitude? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. The value of m indicates the pulse number. <voltage>::=<NRf>[<units>] Where: <NRf> is the amplitude value. <units>::=[mV   V] MINimum queries the minimum amplitude value. MAXimum queries the maximum amplitude voltage.
<b>Returns</b>	<voltage>
<b>Example</b>	SOURce1:DOUBLEPULSe:PULSe1:AMPLitude 2 Set the pulse 1 amplitude value of channel 1 to 2 V.

<b>Command</b>	[SOURce[n]]:DOUBLEPULSe:PULSe[m]:TRANSition[:LEADing]
<b>Description</b>	This command sets or queries the leading edge time of the first or the second pulse in the double pulse waveform. Note that the value is about the leading edge between 10% and 90%.  Note: If the carrier is different from Double Pulse, this command and this query cause an error.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:DOUBLEPULSe:PULSe[m]:TRANSition[:LEADing] <seconds> [SOURce[n]]:DOUBLEPULSe:PULSe[m]:TRANSition[:LEADing]? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:DOUBLEPULSe:PULSe[m]:TRANSition:TRAILing
<b>Arguments</b>	The value of n indicates the channel number. The value of m indicates the pulse number. <seconds>::=<NRf>[<units>] Where: <NRf> is the leading edge time of pulse waveform. <units>::=[ns   μs   ms   s] MINimum queries the minimum transition time. MAXimum queries the maximum transition time.
<b>Returns</b>	<seconds>
<b>Example</b>	SOURce1:DOUBLEPULSe:PULSe1:TRANSition:LEADing 100ns Set the first pulse 1 relative to the double pulse of the channel 1 (CH 1) leading edge time to 100 ns

**Table 117: [SOURce[n]]:PULSe:TRANSition[:LEADing]**

<b>Command</b>	[SOURce[n]]:DOUBLEPULSe:PULSe[m]:TRANSition:TRAILing
<b>Description</b>	This command sets or queries the trailing edge time of the first or the second pulse in the double pulse waveform.  Note: If the carrier is different from Double Pulse, this command and this query cause an error. Note that the value is about the leading edge between 10% and 90%. If the carrier is different from Pulse, this command and this query cause an error.
<b>Group</b>	Source

<b>Syntax</b>	[SOURce[n]]:DOUBLEPULSe:PULSe[m]:TRANSition:TRAIling <seconds> [SOURce[n]]:DOUBLEPULSe:PULSe[m]:TRANSition:TRAIling? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:PULSe:TRANSition[:LEADing]
<b>Arguments</b>	The value of n indicates the channel number. The value of m indicates the pulse number. <seconds>::=<NRf><units>. Where: <NRf> is the trailing edge of pulse waveform. <units>::=[ns   μs   ms   s] MINimum queries the minimum delay. MAXimum queries the maximum delay.
<b>Returns</b>	<seconds>
<b>Example</b>	SOURce1:DOUBLEPULSe:PULSe1:TRANSition:TRAIling 200ns Set the trailing edge time of the first pulse to 200 ns.

**Table 118: [SOURce[n]]:PULSe:TRANSition:TRAIling**

<b>Command</b>	[SOURce[n]]:DOUBLEPULSe:PULSe[m]:WIDTh
<b>Description</b>	This command sets or queries the pulse width of the first or of the second pulse in the double pulse waveform for the specified channel. $\text{Pulse Width} = \text{Period} \times \text{Duty Cycle} / 100$ . The pulse width must be less than the period.  If the carrier is different from Double Pulse, this command and this query cause an error.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:DOUBLEPULSe:PULSe1:WIDTh <seconds> [SOURce[n]]:DOUBLEPULSe:PULSe1:WIDTh? [MINimum   MAXimum]
<b>Related Commands</b>	
<b>Arguments</b>	The value of n indicates the channel number. The value of m indicates the pulse number. <seconds>::=<NRf><units> Where: <NRf> is the pulse width. <units>::=[ns   μs   ms   s] MINimum queries the minimum delay. MAXimum queries the maximum delay.
<b>Returns</b>	<width>
<b>Example</b>	SOURce1:DOUBLEPULSe:PULSe1:WIDTh 100ns Set the first pulse waveform width of the double pulse to 100 ns.

**Table 119:[SOURce[n]]:DOUBLEPULSe:PULSe[m]:WIDTh**

<b>Command</b>	[SOURce[n]]:DOUBLEPULSe:PULSe[m]:DELay
<b>Description</b>	<p>This command sets or queries the delay for first or the second pulse in the double pulse waveform.</p> <p>Important Note: the delay of the second pulse is a delta delay relative to the end of the first pulse.</p> <p>If the carrier is different from Double Pulse, this command and this query cause an error.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:DOUBLEPULSe:PULSe[m]:DELay <delay> [SOURce[n]]:DOUBLEPULSe:PULSe[m]:DELay ? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	<p>The value of n indicates the channel number.</p> <p>The value of m indicates the pulse number.</p> <delay>::=<NRf>[<units>] Where: <NRf> is the initial delay value. <units>::=[ns   μs   ms   s] MINimum queries the minimum delay. MAXimum queries the maximum delay.
<b>Returns</b>	<delay>
<b>Example</b>	SOURce1:DOUBLEPULSe:PULSe1:DELay 300E-9 Set the delay of the first pulse of the double pulse waveform to 300 ns.

**Table 120:[SOURce[n]]:DOUBLEPULSe:PULSe[m]:WIDTH**

<b>Command</b>	[SOURce[n]]:COUPLE:STATe
<b>Description</b>	This command enables or disables the channels coupling between the selected channel and the CH1.  Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:STATe { ON   OFF   0   1} [SOURce[n]]:COUPLE:STATe?
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number and n must be greater than 1. ON   1 enables the channels coupling. OFF   0 disables the channels coupling.
<b>Returns</b>	<NR1> 0 means channels coupling disabled, 1 means channels coupling enabled.
<b>Example</b>	SOURce2:COUPLE:STATe ON Enable the channels coupling between the CH2 and the CH1.

**Table 121: [SOURce[n]]:COUPLE:STATe**

<b>Command</b>	[SOURce[n]]:COUPLE:AMPLitude:STATe
<b>Description</b>	This command enables or disables the channel coupling for the amplitude parameter.  Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this commmand to select the parameter that you want to couple.  Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:AMPLitude:STATe { ON   OFF   0   1} [SOURce[n]]:COUPLE:AMPLitude:STATe?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATe

<b>Arguments</b>	The value of n indicates the channel number and n must be greater than 1. ON   1 enables the channels coupling for the amplitude parameter. OFF   0 disables the channels coupling for the amplitude parameter.
<b>Returns</b>	<NR1> 0 means channel coupling for the amplitude parameter is disabled, 1 means channels coupling for the amplitude parameter is enabled.
<b>Example</b>	SOURce2:COUPLE:STATe ON Enable the channels coupling between the CH2 and the CH1. SOURce2:COUPLE:AMPLitude:STATe ON Enable the channels coupling for the amplitude parameter

**Table 122: [SOURce[n]]:COUPLE:AMPLitude:STATe**

<b>Command</b>	[SOURce[n]]:COUPLE:AMPLitude:RATio
<b>Description</b>	This command sets or queries the ratio for the amplitude parameter in coupling mode.  The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).  The equation of the channel coupling is the following: CHN Parameter = CH1 Parameter*Ratio + Offset.  This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:AMPLitude:RATio <ratio> [SOURce[n]]:COUPLE:AMPLitude:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:AMPLitude:OFFSet
<b>Arguments</b>	The value of n indicates the channel number. n must be greater than 1. <ratio>::=<NRf> Where: <NRf> is the ratio. MINimum queries the minimum ratio. MAXimum queries the maximum ratio. The default is 1.

<b>Returns</b>	<ratio>
<b>Example</b>	SOURce2:COUPLE:AMPLitude:RATio 2.5 Set the amplitude ratio to 2.5

**Table 123: [SOURce[n]]:COUPLE:AMPLitude:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:AMPLitude:OFFSet
<b>Description</b>	<p>This command sets or queries the offset for the amplitude parameter in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following: CHN Parameter = CH1 Parameter*Ratio + Offset.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:AMPLitude:OFFSet <offset> [SOURce[n]]:COUPLE:AMPLitude:OFFSet? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:AMPLitude:RATio
<b>Arguments</b>	<p>The value of n indicates the channel number. n must be greater than 1.</p> <p>&lt;offset&gt;::=&lt;NRf&gt;[&lt;units&gt;] Where: &lt;NRf&gt; is the offset. &lt;units&gt;::=[mV   V]</p> <p>MINimum queries the minimum offset. MAXimum queries the maximum offset. The default is 0.</p>
<b>Returns</b>	<offset>
<b>Example</b>	SOURce2:COUPLE:AMPLitude:OFFSet 1.5 Set the Offset for the amplitude parameter to 1.5 V

**Table 124: [SOURce[n]]:COUPLE:AMPLitude:OFFSet**

<b>Command</b>	[SOURce[n]]:COUPLE:OFFSet:STATe
<b>Description</b>	<p>This command enables or disables the channel coupling for the offset parameter.</p> <p>Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this commmand to select the parameter that you want to couple.</p> <p>Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:OFFSet:STATe { ON   OFF   0   1 } [SOURce[n]]:COUPLE:OFFSet:STATe?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATe
<b>Arguments</b>	<p>The value of n indicates the channel number and n must be greater than 1.</p> <p>ON   1 enables the channels coupling for the offset parameter.</p> <p>OFF   0 disables the channels coupling for the offset parameter.</p>
<b>Returns</b>	<p>&lt;NR1&gt;</p> <p>0 means channel coupling for the offset parameter is disabled, 1 means channels coupling for the offset parameter is enabled.</p>
<b>Example</b>	<p>SOURce2:COUPLE:STATe ON Enable the channels coupling between the CH2 and the CH1.</p> <p>SOURce2:COUPLE:OFFSet:STATe ON Enable the channels coupling for the offset parameter</p>

**Table 125: [SOURce[n]]:COUPLE:OFFSet:STATe**

<b>Command</b>	[SOURce[n]]:COUPLE:OFFSet:RATIo
<b>Description</b>	<p>This command sets or queries the ratio for the offset parameter in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p>



	<p>The equation of the channel coupling is the following:  <math>\text{CHN Parameter} = \text{CH1 Parameter} * \text{Ratio} + \text{Offset}</math>.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:OFFSet:RATio <ratio> [SOURce[n]]:COUPLE:OFFSet:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:OFFSet:OFFSet
<b>Arguments</b>	<p>The value of n indicates the channel number.  n must be greater than 1.  &lt;ratio&gt;::=&lt;NRf&gt; Where: &lt;NRf&gt; is the ratio.  MINimum queries the minimum ratio.  MAXimum queries the maximum ratio.  The default is 1.</p>
<b>Returns</b>	<ratio>
<b>Example</b>	SOURce2:COUPLE:OFFSet:RATio 2.5 Set the offset ratio to 2.5

**Table 126: [SOURce[n]]:COUPLE:OFFSet:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:OFFSet:OFFSet
<b>Description</b>	<p>This command sets or queries the offset for the offset parameter in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  <math>\text{CHN Parameter} = \text{CH1 Parameter} * \text{Ratio} + \text{Offset}</math>.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source

<b>Syntax</b>	[SOURce[n]]:COUPLE:OFFSet:OFFSet <offset> [SOURce[n]]:COUPLE:OFFSet:OFFSet? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:OFFSet:RATio
<b>Arguments</b>	The value of n indicates the channel number. n must be greater than 1. <offset>::=<NRf>[<units>] Where: <NRf> is the offset. <units>::=[mV   V] MINimum queries the minimum offset. MAXimum queries the maximum offset. The default is 0.
<b>Returns</b>	<offset>
<b>Example</b>	SOURce2:COUPLE:OFFSet:OFFSet 2 Set the Offset for the offset parameter to 2 V

**Table 127: [SOURce[n]]:COUPLE:OFFSet:OFFSet**

<b>Command</b>	[SOURce[n]]:COUPLE:FREQuency:STATe
<b>Description</b>	This command enables or disables the channel coupling for the frequency parameter.  Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this commmand to select the parameter that you want to couple.  Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:FREQuency:STATe { ON   OFF   0   1 } [SOURce[n]]:COUPLE:FREQuency:STATe?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATe
<b>Arguments</b>	The value of n indicates the channel number and n must be greater than 1. ON   1 enables the channels coupling for the offset parameter. OFF   0 disables the channels coupling for the offset parameter.
<b>Returns</b>	<NR1>

	0 means channel coupling for the frequency parameter is disabled, 1 means channels coupling for the frequency parameter is enabled.
<b>Example</b>	SOURce2:COUPLE:STATe ON Enable the channels coupling between the CH2 and the CH1. SOURce2:COUPLE:FREQUency:STATe ON Enable the channels coupling for the frequency parameter

**Table 128: [SOURce[n]]:COUPLE:FREQUency:STATe**

<b>Command</b>	[SOURce[n]]:COUPLE:FREQUency:RATio
<b>Description</b>	This command sets or queries the ratio for the frequency parameter in coupling mode.  The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).  The equation of the channel coupling is the following: CHN Parameter = CH1 Parameter*Ratio + Offset.  This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:FREQUency:RATio <ratio> [SOURce[n]]:COUPLE:FREQUency:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:FREQUency:OFFSet
<b>Arguments</b>	The value of n indicates the channel number. n must be greater than 1. <ratio>::=<NRf> Where: <NRf> is the ratio. MINimum queries the minimum ratio. MAXimum queries the maximum ratio. The default is 1.
<b>Returns</b>	<ratio>
<b>Example</b>	SOURce2:COUPLE:FREQUency:RATio 2.5 Set the frequency ratio to 2.5

**Table 129: [SOURce[n]]:COUPLE:FREQUency:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:FREQUENCY:OFFSet
<b>Description</b>	<p>This command sets or queries the offset for the frequency parameter in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  CHN Parameter = CH1 Parameter*Ratio + Offset.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:FREQUENCY:OFFSet <offset> [SOURce[n]]:COUPLE:FREQUENCY:OFFSet? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:FREQUENCY:RATio
<b>Arguments</b>	<p>The value of n indicates the channel number.  n must be greater than 1.  &lt;offset&gt;::=&lt;NRf&gt;[&lt;units&gt;] Where: &lt;NRf&gt; is the offset.  &lt;units&gt;::=[Hz   kHz   MHz].  MINimum queries the minimum offset.  MAXimum queries the maximum offset.  The default is 0.</p>
<b>Returns</b>	<offset>
<b>Example</b>	SOURce2:COUPLE:FREQUENCY:OFFSet 1MHz Set the Offset for the frequency parameter to 1 MHz

**Table 130: [SOURce[n]]:COUPLE:FREQUENCY:OFFSet**

<b>Command</b>	[SOURce[n]]:COUPLE:PHASe:STATe
<b>Description</b>	<p>This command enables or disables the channel coupling for the phase parameter.</p> <p>Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this commmand to select the parameter that you want to couple.</p> <p>Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:PHASe:STATe { ON   OFF   0   1} [SOURce[n]]:COUPLE:PHASe:STATe?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATe
<b>Arguments</b>	<p>The value of n indicates the channel number and n must be greater than 1.</p> <p>ON   1 enables the channels coupling for the offset parameter.</p> <p>OFF   0 disables the channels coupling for the offset parameter.</p>
<b>Returns</b>	<p>&lt;NR1&gt;</p> <p>0 means channel coupling for the phase parameter is disabled, 1 means channels coupling for the phase parameter is enabled.</p>
<b>Example</b>	<p>SOURce2:COUPLE:STATe ON</p> <p>Enable the channels coupling between the CH2 and the CH1.</p> <p>SOURce2:COUPLE: PHASe:STATe ON</p> <p>Enable the channels coupling for the phase parameter</p>

**Table 131: [SOURce[n]]:COUPLE:PHASe:STATe**

<b>Command</b>	[SOURce[n]]:COUPLE:PHASe:RATio
<b>Description</b>	<p>This command sets or queries the ratio for the phase parameter in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p>

	<p>The equation of the channel coupling is the following:  <math>\text{CHN Parameter} = \text{CH1 Parameter} * \text{Ratio} + \text{Offset}</math>.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:PHASe:RATio <ratio> [SOURce[n]]:COUPLE:PHASe:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:PHASe:OFFSet
<b>Arguments</b>	<p>The value of n indicates the channel number.  n must be greater than 1.  &lt;ratio&gt;::=&lt;NRf&gt; Where: &lt;NRf&gt; is the ratio.  MINimum queries the minimum ratio.  MAXimum queries the maximum ratio.  The default is 1.</p>
<b>Returns</b>	<ratio>
<b>Example</b>	SOURce2:COUPLE:PHASe:RATio 2.5 Set the phase ratio to 2.5

**Table 132: [SOURce[n]]:COUPLE:PHASe:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:PHASe:OFFSet
<b>Description</b>	<p>This command sets or queries the offset for the phase parameter in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  <math>\text{CHN Parameter} = \text{CH1 Parameter} * \text{Ratio} + \text{Offset}</math>.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source

<b>Syntax</b>	[SOURce[n]]:COUPLE:PHASe:OFFSet <offset> [SOURce[n]]:COUPLE:PHASe:OFFSet? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:PHASe:RATio
<b>Arguments</b>	The value of n indicates the channel number. n must be greater than 1. <offset>::=<NR3><units>] Where:<NR3> is the offset. <units>::=[°   DEG]. MINimum queries the minimum offset. MAXimum queries the maximum offset. The default is 0.
<b>Returns</b>	<offset>
<b>Example</b>	SOURce2:COUPLE:PHASe:OFFSet 10DEG Set the Offset for the phase parameter to 10 degrees.

**Table 133: [SOURce[n]]:COUPLE:PHASe:OFFSet**

<b>Command</b>	[SOURce[n]]:COUPLE:DCYCLe:STATe
<b>Description</b>	This command enables or disables the channel coupling for the duty cycle parameter.  Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this command to select the parameter that you want to couple.  Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DCYCLe:STATe { ON   OFF   0   1} [SOURce[n]]:COUPLE: DCYCLe:STATe?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATe
<b>Arguments</b>	The value of n indicates the channel number and n must be greater than 1. ON   1 enables the channels coupling for the offset parameter. OFF   0 disables the channels coupling for the offset parameter.
<b>Returns</b>	<NR1> 0 means channel coupling for the duty cycle parameter is disabled, 1 means channels coupling for the duty cycle parameter is enabled.

<b>Example</b>	<p>SOURce2:COUPLE:STATe ON  Enable the channels coupling between the CH2 and the CH1.</p> <p>SOURce2:COUPLE:DCYCLe:STATe ON  Enable the channels coupling for the duty cycle parameter</p>
----------------	--

**Table 134: [SOURce[n]]:COUPLE:DCYCLe:STATe**

<b>Command</b>	[SOURce[n]]:COUPLE:DCYCLe:RATio
<b>Description</b>	<p>This command sets or queries the ratio for the duty cycle parameter in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  CHN Parameter = CH1 Parameter*Ratio + Offset.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DCYCLe:RATio <ratio> [SOURce[n]]:COUPLE:DCYCLe:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:DCYCLe:OFFSet
<b>Arguments</b>	<p>The value of n indicates the channel number.  n must be greater than 1.</p> <p>&lt;ratio&gt;::=&lt;NRf&gt; Where: &lt;NRf&gt; is the ratio.  MINimum queries the minimum ratio.  MAXimum queries the maximum ratio.  The default is 1.</p>
<b>Returns</b>	<ratio>
<b>Example</b>	<p>SOURce2:COUPLE:DCYCLe:RATio 2.5  Set the frequency duty cycle to 2.5</p>

**Table 135: [SOURce[n]]:COUPLE:DCYCLe:RATio**



<b>Command</b>	[SOURce[n]]:COUPLE:DCYCLe:OFFSet
<b>Description</b>	<p>This command sets or queries the offset for the duty cycle parameter in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  <math>CHN \text{ Parameter} = CH1 \text{ Parameter} * \text{Ratio} + \text{Offset}</math>.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DCYCLe:OFFSet <offset> [SOURce[n]]:COUPLE:DCYCLe:OFFSet? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:DCYCLe:RATio
<b>Arguments</b>	<p>The value of n indicates the channel number.  n must be greater than 1.  &lt;offset&gt;::=&lt;NR2&gt;[&lt;units&gt;] Where: &lt;NR2&gt; is the offset.  &lt;units&gt;::=PCT  MINimum queries the minimum offset.  MAXimum queries the maximum offset.  The default is 0.</p>
<b>Returns</b>	<offset>
<b>Example</b>	SOURce2:COUPLE:DCYCLe:OFFSet 10.5 Set the Offset for the duty cycle parameter to 10.5 %

**Table 136: [SOURce[n]]:COUPLE:DCYCLe:OFFSet**

<b>Command</b>	[SOURce[n]]:COUPLE:LEADIng:STATe
<b>Description</b>	<p>This command enables or disables the channel coupling for the leading edge parameter.</p> <p>Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this commmand to select the parameter that you want to couple.</p> <p>Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:LEADIng:STATe { ON   OFF   0   1 } [SOURce[n]]:COUPLE:LEADIng:STATe?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATe
<b>Arguments</b>	<p>The value of n indicates the channel number and n must be greater than 1.</p> <p>ON 1 enables the channels coupling for the leading edge parameter.</p> <p>OFF 0 disables the channels coupling for the leading edge parameter.</p>
<b>Returns</b>	<p>&lt;NR1&gt;</p> <p>0 means channel coupling for the leading edge parameter is disabled, 1 means channels coupling for the leading edge parameter is enabled.</p>
<b>Example</b>	<p>SOURce2:COUPLE:STATe ON</p> <p>Enable the channels coupling between the CH2 and the CH1.</p> <p>SOURce2:COUPLE:LEADIng:STATe ON</p> <p>Enable the channels coupling for the leading edge parameter</p>

**Table 137: [SOURce[n]]:COUPLE:LEADIng:STATe**

<b>Command</b>	[SOURce[n]]:COUPLE:LEADing:RATio
<b>Description</b>	<p>This command sets or queries the ratio for the leading edge parameter in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following: CHN Parameter = CH1 Parameter*Ratio + Offset.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:LEADing:RATio <ratio> [SOURce[n]]:COUPLE:LEADing:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:LEADing:OFFSet
<b>Arguments</b>	<p>The value of n indicates the channel number. n must be greater than 1. &lt;ratio&gt;::=&lt;NRf&gt; Where: &lt;NRf&gt; is the ratio. MINimum queries the minimum ratio. MAXimum queries the maximum ratio. The default is 1.</p>
<b>Returns</b>	<ratio>
<b>Example</b>	SOURce2:COUPLE:LEADing:RATio 2.5 Set the leading edge ratio to 2.5

**Table 138: [SOURce[n]]:COUPLE:LEADing:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:LEADing:OFFSet
<b>Description</b>	This command sets or queries the offset for the leading edge parameter in coupling mode.

	<p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  <math>CHN \text{ Parameter} = CH1 \text{ Parameter} * \text{Ratio} + \text{Offset}</math>.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:LEADing:OFFSet <offset> [SOURce[n]]:COUPLE:LEADing:OFFSet? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:LEADing:RATio
<b>Arguments</b>	<p>The value of n indicates the channel number.  n must be greater than 1.  &lt;offset&gt;::=&lt;NRf&gt;[&lt;units&gt;] Where: &lt;NRf&gt; is the offset.  &lt;units&gt;::=[ns   μs   ms   s].  MINimum queries the minimum offset.  MAXimum queries the maximum offset.  The default is 0.</p>
<b>Returns</b>	<offset>
<b>Example</b>	SOURce2:COUPLE:LEADing:OFFSet 10ns Set the Offset for the leading edge parameter to 10 ns.

**Table 139: [SOURce[n]]:COUPLE:LEADing:OFFSet**

<b>Command</b>	[SOURce[n]]:COUPLE:TRAILing:STATe
<b>Description</b>	<p>This command enables or disables the channel coupling for the trailing edge parameter.</p> <p>Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this commmand to select the parameter that you want to couple.</p> <p>Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.</p>

<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:TRAILing:STATe { ON   OFF   0   1} [SOURce[n]]:COUPLE:TRAILing:STATe?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATe
<b>Arguments</b>	The value of n indicates the channel number and n must be greater than 1. ON 1 enables the channels coupling for the trailing edge parameter. OFF 0 disables the channels coupling for the trailing edge parameter.
<b>Returns</b>	<NR1> 0 means channel coupling for the trailing edge parameter is disabled, 1 means channels coupling for the trailing edge parameter is enabled.
<b>Example</b>	SOURce2:COUPLE:STATe ON Enable the channels coupling between the CH2 and the CH1. SOURce2:COUPLE:TRAILing:STATe ON Enable the channels coupling for the trailing edge parameter

**Table 140: [SOURce[n]]:COUPLE:TRAILing:STATe**

<b>Command</b>	[SOURce[n]]:COUPLE:TRAILing:RATio
<b>Description</b>	This command sets or queries the ratio for the trailing edge parameter in coupling mode.  The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).  The equation of the channel coupling is the following: CHN Parameter = CH1 Parameter*Ratio + Offset.  This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.
<b>Group</b>	Source

<b>Syntax</b>	[SOURce[n]]:COUPLE:TRAILing:RATio <ratio> [SOURce[n]]:COUPLE:TRAILing:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:TRAILing:OFFSet
<b>Arguments</b>	The value of n indicates the channel number. n must be greater than 1. <ratio>::=<NRf> Where: <NRf> is the ratio. MINimum queries the minimum ratio. MAXimum queries the maximum ratio. The default is 1.
<b>Returns</b>	<ratio>
<b>Example</b>	SOURce2:COUPLE:TRAILing:RATio 2.5 Set the trailing edge ratio to 2.5

**Table 141: [SOURce[n]]:COUPLE:LEADing:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:TRAILing:OFFSet
<b>Description</b>	This command sets or queries the offset for the trailing edge parameter in coupling mode.  The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).  The equation of the channel coupling is the following: CHN Parameter = CH1 Parameter*Ratio + Offset.  This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:TRAILing:OFFSet <offset> [SOURce[n]]:COUPLE:TRAILing:OFFSet? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:TRAILing:RATio
<b>Arguments</b>	The value of n indicates the channel number. n must be greater than 1. <offset>::=<NRf>[<units>] Where: <NRf> is the offset. <units>::=[ns   μs   ms   s]. MINimum queries the minimum offset.

	MAXimum queries the maximum offset. The default is 0.
<b>Returns</b>	<offset>
<b>Example</b>	SOURce2:COUPLE:TRAIling:OFFSet 10ns Set the Offset for the trailing edge parameter to 10 ns.

**Table 142: [SOURce[n]]:COUPLE:TRAIling:OFFSet**

<b>Command</b>	[SOURce[n]]:COUPLE:SYMMetry:STATe
<b>Description</b>	This command enables or disables the channel coupling for the ramp symmetry parameter.  Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this commmand to select the parameter that you want to couple.  Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:SYMMetry:STATe { ON   OFF   0   1} [SOURce[n]]:COUPLE:SYMMetry:STATe?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATe
<b>Arguments</b>	The value of n indicates the channel number and n must be greater than 1. ON 1 enables the channels coupling for the ramp symmetry parameter. OFF 0 disables the channels coupling for the ramp symmetry parameter.
<b>Returns</b>	<NR1> 0 means channel coupling for the ramp symmetry parameter is disabled, 1 means channels coupling for the ramp symmetry parameter is enabled.
<b>Example</b>	SOURce2:COUPLE:STATe ON Enable the channels coupling between the CH2 and the CH1. SOURce2:COUPLE:SYMMetry:STATe ON Enable the channels coupling for the ramp symmetry parameter

**Table 143: [SOURce[n]]:COUPLE:SYMMetry:STATe**

<b>Command</b>	[SOURce[n]]:COUPLE:SYMMetry:RATio
<b>Description</b>	<p>This command sets or queries the ratio for the ramp symmetry parameter in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following: CHN Parameter = CH1 Parameter*Ratio + Offset.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:SYMMetry:RATio <ratio> [SOURce[n]]:COUPLE:SYMMetry:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:SYMMetry:OFFSet
<b>Arguments</b>	<p>The value of n indicates the channel number. n must be greater than 1. &lt;ratio&gt;::=&lt;NRf&gt; Where: &lt;NRf&gt; is the ratio. MINimum queries the minimum ratio. MAXimum queries the maximum ratio. The default is 1.</p>
<b>Returns</b>	<ratio>
<b>Example</b>	SOURce2:COUPLE:SYMMetry:RATio 2.5 Set the ramp symmetry ratio to 2.5

**Table 144: [SOURce[n]]:COUPLE:SYMMetry:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:SYMMetry:OFFSet
<b>Description</b>	This command sets or queries the offset for the ramp symmetry parameter in coupling mode.



	<p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  <math>CHN \text{ Parameter} = CH1 \text{ Parameter} * \text{Ratio} + \text{Offset}</math>.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:SYMMetry:OFFSet <offset> [SOURce[n]]:COUPLE:SYMMetry:OFFSet? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:SYMMetry:RATio
<b>Arguments</b>	<p>The value of n indicates the channel number.  n must be greater than 1.  &lt;offset&gt;::=&lt;NR2&gt;[&lt;units&gt;] Where: &lt;NR2&gt; is the offset.  &lt;units&gt;::=PCT  MINimum queries the minimum offset.  MAXimum queries the maximum offset.  The default is 0.</p>
<b>Returns</b>	<offset>
<b>Example</b>	SOURce2:COUPLE:SYMMetry:OFFSet 20.5% Set the Offset for the trailing edge parameter to 20.5 %.

**Table 145: [SOURce[n]]:COUPLE:SYMMetry:OFFSet**

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:AMPLitude:STATe
<b>Description</b>	<p>This command enables or disables the channel coupling for the amplitude parameter of the double pulse waveform.</p> <p>Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this command to select the parameter that you want to couple.</p>

	Note: if [SOURCE[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.
<b>Group</b>	Source
<b>Syntax</b>	[SOURCE[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLITUDE:STATE { ON   OFF   0   1 } [SOURCE[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLITUDE:STATE?
<b>Related Commands</b>	[SOURCE[n]]:COUPLE:STATE
<b>Arguments</b>	The value of n indicates the channel number and n must be greater than 1. The value of m indicates the pulse number. ON   1 enables the channels coupling for the amplitude parameter of the double pulse waveform. OFF   0 disables the channels coupling for the amplitude parameter of the double pulse waveform.
<b>Returns</b>	<NR1> 0 means channel coupling for the double pulse amplitude parameter is disabled, 1 means channels coupling for the double pulse amplitude parameter is enabled.
<b>Example</b>	SOURCE2:COUPLE:STATE ON Enable the channels coupling between the CH2 and the CH1. SOURCE2:COUPLE:DOUBLEPULSE:PULSE1:AMPLITUDE:STATE ON Enable the channels coupling for the Pulse 1 amplitude parameter of the double pulse waveform.

**Table 146: [SOURCE[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLITUDE:STATE**

<b>Command</b>	[SOURCE[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLITUDE:RATIO
<b>Description</b>	This command sets or queries the ratio for the double pulse amplitude parameter in coupling mode.  The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).  The equation of the channel coupling is the following: CHN Parameter = CH1 Parameter*Ratio + Offset.

	This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLitude:RATio <ratio> [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLitude:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLitude:OFFSet
<b>Arguments</b>	The value of n indicates the channel number. n must be greater than 1. The value of m indicates the pulse number. <ratio>::=<NRf> Where: <NRf> is the ratio. MINimum queries the minimum ratio. MAXimum queries the maximum ratio. The default is 1.
<b>Returns</b>	<ratio>
<b>Example</b>	SOURce2:COUPLE:DOUBLEPULSE:PULSE1:AMPLitude:RATio 2.5 Set the Pulse 1 amplitude ratio of the double pulse waveform to 2.5

**Table 147: [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLitude:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLitude:OFFSet
<b>Description</b>	This command sets or queries the offset for the double pulse amplitude parameter in coupling mode.  The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).  The equation of the channel coupling is the following: CHN Parameter = CH1 Parameter*Ratio + Offset.  This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.
<b>Group</b>	Source

<b>Syntax</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLitude:OFFSet <offset> [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLitude:OFFSet? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLitude:RATio
<b>Arguments</b>	The value of n indicates the channel number. n must be greater than 1. The value of m indicates the pulse number. <offset>::=<NRf><units>] Where: <NRf> is the offset. <units>::=[mV   V] MINimum queries the minimum offset. MAXimum queries the maximum offset. The default is 0.
<b>Returns</b>	<offset>
<b>Example</b>	SOURce2:COUPLE:DOUBLEPULSE:PULSE1:AMPLitude:OFFSet 1.5 Set the Pulse 1 Offset for the double pulse amplitude parameter to 1.5 V

Table 148: [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:AMPLitude:OFFSet

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:LEADing:STATe
<b>Description</b>	This command enables or disables the channel coupling for the leading edge parameter of the double pulse waveform.  Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this commmand to select the parameter that you want to couple.  Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:LEADing:STATe { ON   OFF   0   1} [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:LEADing:STATe?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATe
<b>Arguments</b>	The value of n indicates the channel number and n must be greater than 1.

	<p>The value of m indicates the pulse number.</p> <p>ON 1 enables the channels coupling for the leading edge parameter of the double pulse waveform.</p> <p>OFF 0 disables the channels coupling for the leading edge parameter of the double pulse waveform.</p>
<b>Returns</b>	<p>&lt;NR1&gt;</p> <p>0 means channel coupling for the double pulse leading edge parameter is disabled, 1 means channels coupling for the double pulse leading edge parameter is enabled.</p>
<b>Example</b>	<p>SOURce2:COUPLE:STATE ON</p> <p>Enable the channels coupling between the CH2 and the CH1.</p> <p>SOURce2:DOUBLEPULSE:PULSE1:LEADing:STATE ON</p> <p>Enable the channels coupling for the Pulse 1 leading edge parameter of the double pulse waveform.</p>

**Table 149: Command [SOURCE[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:LEADing:STATE**

<b>Command</b>	[SOURCE[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:LEADing:RATio
<b>Description</b>	<p>This command sets or queries the ratio for the leading edge parameter of the double pulse waveform in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  <math>CHN \text{ Parameter} = CH1 \text{ Parameter} * \text{Ratio} + \text{Offset}</math>.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	<p>[SOURCE[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:LEADing:RATio &lt;ratio&gt;</p> <p>[SOURCE[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:LEADing:RATio?</p> <p>[MINimum   MAXimum]</p>
<b>Related Commands</b>	[SOURCE[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:LEADing:OFFSet
<b>Arguments</b>	The value of n indicates the channel number.

	<p>n must be greater than 1.  The value of m indicates the pulse number.  &lt;ratio&gt;::=&lt;NRf&gt; Where: &lt;NRf&gt; is the ratio.  MINimum queries the minimum ratio.  MAXimum queries the maximum ratio.  The default is 1.</p>
<b>Returns</b>	<ratio>
<b>Example</b>	<p>SOURce2:COUPLE:DOUBLEPULSe:PULSe1:LEADing:RATio 2.5  Set the Pulse 1 leading edge ratio of the double pulse waveform to 2.5</p>

**Table 150: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:OFFSet
<b>Description</b>	<p>This command sets or queries the offset for the leading edge parameter of the double pulse waveform in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  CHN Parameter = CH1 Parameter*Ratio + Offset.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	<p>[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:OFFSet  &lt;offset&gt;  [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:OFFSet?  [MINimum   MAXimum]</p>
<b>Related Commands</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:LEADing:RATio
<b>Arguments</b>	<p>The value of n indicates the channel number.  n must be greater than 1.  The value of m indicates the pulse number.  &lt;offset&gt;::=&lt;NRf&gt;[&lt;units&gt;] Where: &lt;NRf&gt; is the offset.  &lt;units&gt;::=[ns   μs   ms   s].</p>

	MINimum queries the minimum offset. MAXimum queries the maximum offset. The default is 0.
<b>Returns</b>	<offset>
<b>Example</b>	SOURce2:COUPLE:DOUBLEPULSE:PULSE1:LEADing:OFFSet 10ns Set the Offset for the Pulse 1 leading edge parameter of the double pulse waveform to 10 ns.

**Table 151: [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:LEADing:OFFSet**

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:TRAILing:STATe
<b>Description</b>	<p>This command enables or disables the channel coupling for the trailing edge parameter of the double pulse waveform.</p> <p>Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this commmand to select the parameter that you want to couple.</p> <p>Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:TRAILing:STATe { ON   OFF   0   1} [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:TRAILing:STATe?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATe
<b>Arguments</b>	<p>The value of n indicates the channel number and n must be greater than 1.</p> <p>The value of m indicates the pulse number.</p> <p>ON   1 enables the channels coupling for the trailing edge parameter of the double pulse waveform.</p> <p>OFF   0 disables the channels coupling for the trailing edge parameter of the double pulse waveform.</p>
<b>Returns</b>	<NR1>

	0 means channel coupling for the double pulse trailing edge parameter is disabled, 1 means channels coupling for the double pulse trailing edge parameter is enabled.
<b>Example</b>	<p>SOURce2:COUPLE:STATe ON  Enable the channels coupling between the CH2 and the CH1.</p> <p>SOURce2:DOUBLEPULSe:PULSe1:TRAILing:STATe ON  Enable the channels coupling for the Pulse 1 trailing edge parameter of the double pulse waveform.</p>

**Table 152: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAILing:STATe**

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAILing:RATio
<b>Description</b>	<p>This command sets or queries the ratio for the trailing edge parameter of the double pulse waveform in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  CHN Parameter = CH1 Parameter*Ratio + Offset.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAILing:RATio <ratio> [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAILing:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAILing:OFFSet
<b>Arguments</b>	<p>The value of n indicates the channel number.  n must be greater than 1.</p> <p>The value of m indicates the pulse number.</p> <p>&lt;ratio&gt;::=&lt;NRf&gt; Where: &lt;NRf&gt; is the ratio.</p> <p>MINimum queries the minimum ratio.  MAXimum queries the maximum ratio.</p>



	The default is 1.
<b>Returns</b>	<ratio>
<b>Example</b>	SOURce2:COUPLE:DOUBLEPULSe:PULSe1:TRAIling:RATio 2.5 Set the Pulse 1 trailing edge ratio of the double pulse waveform to 2.5

**Table 153: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:OFFSet
<b>Description</b>	<p>This command sets or queries the offset for the trailing edge parameter of the double pulse waveform in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following: CHN Parameter = CH1 Parameter*Ratio + Offset.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:OFFSet <offset> [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:OFFSet? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:TRAIling:RATio
<b>Arguments</b>	<p>The value of n indicates the channel number. n must be greater than 1.</p> <p>The value of m indicates the pulse number.</p> <p>&lt;offset&gt;::=&lt;NRf&gt;[&lt;units&gt;] Where: &lt;NRf&gt; is the offset. &lt;units&gt;::=[ns   μs   ms   s].</p> <p>MINimum queries the minimum offset. MAXimum queries the maximum offset.</p> <p>The default is 0.</p>
<b>Returns</b>	<offset>

<b>Example</b>	SOURce2:COUPLE:DOUBLEPULSe:PULSe1:TRAIling:OFFSet 10ns Set the Offset for the Pulse 1 trailing edge parameter of the double pulse waveform to 10 ns.
----------------	---

**Table 154: [SOURce[n]]:COUPLE:LEADing:OFFSet**

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:STATe
<b>Description</b>	This command enables or disables the channel coupling for the width parameter of the double pulse waveform.  Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATe command, you have to use this commmand to select the parameter that you want to couple.  Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:STATe { ON   OFF   0   1} [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:STATe?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATe
<b>Arguments</b>	The value of n indicates the channel number and n must be greater than 1. The value of m indicates the pulse number. ON   1 enables the channels coupling for the width parameter of the double pulse waveform. OFF   0 disables the channels coupling for the width parameter of the double pulse waveform.
<b>Returns</b>	<NR1> 0 means channel coupling for the double pulse width parameter is disabled, 1 means channels coupling for the double pulse width parameter is enabled.
<b>Example</b>	SOURce2:COUPLE:STATe ON Enable the channels coupling between the CH2 and the CH1. SOURce2:COUPLE:DOUBLEPULSe:PULSe1:WIDTh:STATe ON Enable the channels coupling for the Pulse 1 trailing edge parameter of the double pulse waveform.

**Table 155: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:STATe**

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:RATio
<b>Description</b>	<p>This command sets or queries the ratio for the width edge parameter of the double pulse waveform in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following: CHN Parameter = CH1 Parameter*Ratio + Offset.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:RATio <ratio> [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:OFFSet
<b>Arguments</b>	<p>The value of n indicates the channel number. n must be greater than 1.</p> <p>The value of m indicates the pulse number.</p> <p>&lt;ratio&gt;::=&lt;NRf&gt; Where: &lt;NRf&gt; is the ratio.</p> <p>MINimum queries the minimum ratio.</p> <p>MAXimum queries the maximum ratio.</p> <p>The default is 1.</p>
<b>Returns</b>	<ratio>
<b>Example</b>	SOURce2:COUPLE:DOUBLEPULSe:PULSe1:WIDTh:RATio 2.5 Set the Pulse 1 width ratio of the double pulse waveform to 2.5

**Table 156: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:OFFSet
<b>Description</b>	This command sets or queries the offset for the width parameter of the double pulse waveform in coupling mode.

	<p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  <math>CHN \text{ Parameter} = CH1 \text{ Parameter} * \text{Ratio} + \text{Offset}</math>.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	<pre>[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:OFFSet &lt;offset&gt; [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:OFFSet? [MINimum   MAXimum]</pre>
<b>Related Commands</b>	<pre>[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:RATio</pre>
<b>Arguments</b>	<p>The value of n indicates the channel number.  n must be greater than 1.</p> <p>The value of m indicates the pulse number.  &lt;offset&gt;::=&lt;NRf&gt;[&lt;units&gt;] Where: &lt;NRf&gt; is the offset.  &lt;units&gt;::=[ns   μs   ms   s].</p> <p>MINimum queries the minimum offset.  MAXimum queries the maximum offset.  The default is 0.</p>
<b>Returns</b>	<offset>
<b>Example</b>	<pre>SOURce2:COUPLE:DOUBLEPULSe:PULSe1:WIDTh:OFFSet 10ns</pre> <p>Set the Offset for the Pulse 1 width parameter of the double pulse waveform to 10 ns.</p>

Table 157: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:WIDTh:OFFSet

<b>Command</b>	<pre>[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:DELay:STATe</pre>
<b>Description</b>	This command enables or disables the channel coupling for the delay parameter of the double pulse waveform.

	<p>Once the channel coupling between two channels have been enabled using the [SOURce[n]]:COUPLE:STATE command, you have to use this commmand to select the parameter that you want to couple.</p> <p>Note: if [SOURce[n]] will be omitted the channels coupling will be made between the CH2 and the CH1.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:DELAY:STATE { ON   OFF   0   1} [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:DELAY:STATE?
<b>Related Commands</b>	[SOURce[n]]:COUPLE:STATE
<b>Arguments</b>	<p>The value of n indicates the channel number and n must be greater than 1.</p> <p>The value of m indicates the pulse number.</p> <p>ON   1 enables the channels coupling for the delay parameter of the double pulse waveform.</p> <p>OFF   0 disables the channels coupling for the delay parameter of the double pulse waveform.</p>
<b>Returns</b>	<p>&lt;NR1&gt;</p> <p>0 means channel coupling for the double pulse delay parameter is disabled, 1 means channels coupling for the double pulse delay parameter is enabled.</p>
<b>Example</b>	<p>SOURce2:COUPLE:STATE ON Enable the channels coupling between the CH2 and the CH1.</p> <p>SOURce2:COUPLE:DOUBLEPULSE:PULSE1:DELAY:STATE ON Enable the channels coupling for the Pulse 1 trailing edge parameter of the double pulse waveform.</p>

**Table 158: [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:DELAY:STATE**

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:DELAY:RATIo
<b>Description</b>	This command sets or queries the ratio for the delay parameter of the double pulse waveform in coupling mode.

	<p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p> <p>The equation of the channel coupling is the following:  <math>CHN \text{ Parameter} = CH1 \text{ Parameter} * \text{Ratio} + \text{Offset}</math>.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:DELay:RATio <ratio> [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:DELay:RATio? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:DELay:OFFSet
<b>Arguments</b>	<p>The value of n indicates the channel number.  n must be greater than 1.</p> <p>The value of m indicates the pulse number.  &lt;ratio&gt;::=&lt;NRf&gt; Where: &lt;NRf&gt; is the ratio.  MINimum queries the minimum ratio.  MAXimum queries the maximum ratio.  The default is 1.</p>
<b>Returns</b>	<ratio>
<b>Example</b>	SOURce2:COUPLE:DOUBLEPULSe:PULSe1:DELay:RATio 2.5 Set the Pulse 1 delay of the double pulse waveform to 2.5

**Table 159: [SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:DELay:RATio**

<b>Command</b>	[SOURce[n]]:COUPLE:DOUBLEPULSe:PULSe[m]:DELay:OFFSet
<b>Description</b>	<p>This command sets or queries the offset for the delay parameter of the double pulse waveform in coupling mode.</p> <p>The Channel Coupling allows you to specify that Channel 1 parameter like frequency, amplitude, offset etc. must be related to other channel's parameter by a ratio (multiplying) and an offset (adding).</p>

	<p>The equation of the channel coupling is the following:  <math>CHN \text{ Parameter} = CH1 \text{ Parameter} * Ratio + Offset</math>.</p> <p>This command causes an error when the result of the formula exceeds the ranges of the CHN parameter.</p>
<b>Group</b>	Source
<b>Syntax</b>	<p>[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:DELay:OFFSet          &lt;offset&gt;          [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:DELay:OFFSet?          [MINimum   MAXimum]</p>
<b>Related Commands</b>	[SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:DELay:RATio
<b>Arguments</b>	<p>The value of n indicates the channel number.          n must be greater than 1.          The value of m indicates the pulse number.          &lt;offset&gt;::=&lt;NRf&gt;[&lt;units&gt;] Where: &lt;NRf&gt; is the offset.          &lt;units&gt;::=[ns   μs   ms   s].          MINimum queries the minimum offset.          MAXimum queries the maximum offset.          The default is 0.</p>
<b>Returns</b>	<offset>
<b>Example</b>	<p>SOURce2:COUPLE:DOUBLEPULSE:PULSE1:DELay:OFFSet 10ns          Set the Offset for the Pulse 1 delay parameter of the double pulse waveform to 10 ns.</p>

**Table 160: [SOURce[n]]:COUPLE:DOUBLEPULSE:PULSE[m]:DELay:OFFSet**

<b>Command</b>	[SOURce[n]]:VOLTage:LIMit:HIGH
<b>Description</b>	This command sets or queries the higher limit of the output amplitude high level for the specified channel.
<b>Group</b>	Source
<b>Syntax</b>	<p>[SOURce[n]]:VOLTage:LIMit:HIGH &lt;voltage&gt;          [SOURce[n]]:VOLTage:LIMit:HIGH? [MINimum   MAXimum]</p>
<b>Related Commands</b>	[SOURce[n]]:VOLTage:LIMit:LOW

<b>Arguments</b>	<voltage>::=<NRf>[<units> Where: <NRf> is the higher limit of output amplitude. <units>::=[mV   V] MINimum queries the minimum high limit level. MAXimum queries the maximum high limit level.
<b>Returns</b>	<voltage>
<b>Example</b>	SOURce1:VOLTage:LIMit:HIGH 1V Set the higher limit of channel 1 output amplitude to 1 V.

**Table 161: [SOURce[n]]:VOLTage:LIMit:HIGH**

<b>Command</b>	[SOURce[n]]:VOLTage:LIMit:LOW
<b>Description</b>	This command sets or queries the lower limit of the output amplitude low level for the specified channel.
<b>Group</b>	Source
<b>Syntax</b>	[SOURce[n]]:VOLTage:LIMit:LOW <voltage> [SOURce[n]]:VOLTage:LIMit:LOW? [MINimum   MAXimum]
<b>Related Commands</b>	[SOURce[n]]:VOLTage:LIMit:HIGH
<b>Arguments</b>	<voltage>::=<NRf>[<units> Where: <NRf> is the higher limit of output amplitude. <units>::=[mV   V] MINimum queries the minimum low limit level. MAXimum queries the maximum low limit level.
<b>Returns</b>	<voltage>
<b>Example</b>	SOURce1:VOLTage:LIMit:LOW 10mV Set the lower limit of channel 1 output amplitude to 10 mV.

**Table 162: [SOURce[n]]:VOLTage:LIMit:LOW**



<b>Command</b>	AFGControl:START
<b>Description</b>	This command runs the instrument and starts the generation. There is no query form of this command.
<b>Group</b>	Device Commands
<b>Syntax</b>	AFGControl:START
<b>Related Commands</b>	AFGControl:STOP
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	AFGControl:START Send the start command to the function generator.

**Table 163: AFGControl:START**

<b>Command</b>	AFGControl:STOP
<b>Description</b>	This command stops the instrument. There is no query form of this command.
<b>Group</b>	Device Commands
<b>Syntax</b>	AFGControl:STOP
<b>Related Commands</b>	AFGControl:START
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	AFGControl:STOP Send the stop command to the function generator.

**Table 164: AFGControl:STOP**

<b>Command</b>	AFGControl:STATus (Query only)
<b>Description</b>	This command queries the status of the function generator. This command is query only.
<b>Group</b>	Device Commands
<b>Syntax</b>	AFGControl:STATus?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	0 if the instrument is in stopped state. 1 if the instrument is in run state.
<b>Example</b>	AFGControl:STATus? Return the status of the function generator.

**Table 165: AFGControl:STATus**

<b>Command</b>	AFGControl:COPY
<b>Description</b>	This command copies all parameter data from the source channel to the others.
<b>Group</b>	Device Commands
<b>Syntax</b>	AFGControl:COPY <source channel>
<b>Related Commands</b>	None
<b>Arguments</b>	<source channel>::<=<NR1> Where <NR1> indicates the channel number.
<b>Returns</b>	None
<b>Example</b>	AFGControl:COPY 1 Copies the CH1 parameters into the others channels

**Table 166: AFGControl:COPY**

<b>Command</b>	AFGControl:AWGSwitch
<b>Description</b>	This command allows to switch from AT-Simple-AFG software to AT-True-ARB software.
<b>Group</b>	Device Commands
<b>Syntax</b>	AFGControl:AWGSwitch
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	AFGControl:AWGSwitch Launches the AT-True-ARB software while AT-Simple-AFG is running.

**Table 167: AFGControl:AWGSwitch**

<b>Command</b>	*RST
<b>Description</b>	This command resets the instrument to its default state. There is no query form of this command.
<b>Group</b>	System
<b>Syntax</b>	*RST
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	*RST Resets the instrument.

**Table 168: \*RST**

<b>Command</b>	SYSTem:BEEPer[:IMMEDIATE]
<b>Description</b>	This command causes the instrument to beep immediately. There is no query form of this command.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:BEEPer[:IMMEDIATE]
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	SYSTem:BEEPer:IMMEDIATE Causes an audible beep.

**Table 169: SYSTem:BEEPer[:IMMEDIATE]**

<b>Command</b>	SYSTem:BEEPer:STATe
<b>Description</b>	This command enables or disables the instrument beeper. When the beeper is set to ON, the instrument will beep when an error is caused by remote command execution.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:BEEPer:STATe { ON   OFF   0   1 } SYSTem:BEEPer:STATe?
<b>Related Commands</b>	SYSTem:BEEPer[:IMMEDIATE]
<b>Arguments</b>	ON   1 enables the beeper. OFF   0 disables the beeper.
<b>Returns</b>	<NR1> 1 means that the beeper is enabled, 0 means that it is disabled.
<b>Example</b>	SYSTem:BEEPer:STATe ON Enable the beeper function.

**Table 170: SYSTem:BEEPer:STATe**

<b>Command</b>	SYSTem:ERRor[:NEXT] (Query only)
<b>Description</b>	This command returns the contents of the Error/Event queue. This command is query only.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:ERRor[:NEXT]?
<b>Related Commands</b>	SYSTem:BEEPer[:IMMEDIATE]
<b>Arguments</b>	None
<b>Returns</b>	<NR1>::=<Error/event number>

	<Qstring>::=<Error/event description>
<b>Example</b>	<p>SYSTem:ERRor:NEXt?</p> <p>Example return: “-221, Error on run mode: the AFG is not in the correct run mode for this operation”.</p> <p>If the instrument detects an error or an event occurs, the event number and event message will be returned.</p>

**Table 171: SYSTem:ERRor[:NEXt]**

<b>Command</b>	SYSTem:KCLick[:STATe]
<b>Description</b>	This command enables or disables the key click sound when you push the front panel buttons, turn the general-purpose knob or touch/click a control on the user interface.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:KCLick[:STATe] { ON   OFF   0   1 } SYSTem:KCLick[:STATe]?
<b>Related Commands</b>	ON   1 enables key click sound. OFF   0 disables key click sound.
<b>Arguments</b>	None
<b>Returns</b>	<NR1> 0 means OFF, 1 means ON
<b>Example</b>	SYSTem:KCLick:STATe ON Enable the key click sound.

**Table 172: SYSTem:KCLick[:STATe]**

<b>Command</b>	SYSTem:TLOCK[:STATe]
<b>Description</b>	This command locks or unlocks the touch screen interface. When you set the ON state (lock enabled), the events related to the touch screen will be disabled.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:TLOCK[:STATe] { ON   OFF   0   1 } SYSTem:TLOCK[:STATe]?
<b>Related Commands</b>	None
<b>Arguments</b>	ON locks the user interface. OFF unlocks the user interface.
<b>Returns</b>	<NR1> 1 means that the UI is locked, 0 means that it is unlocked.
<b>Example</b>	SYSTem:TLOCK:STATe ON Lock the user interface.

**Table 173: SYSTem:TLOCK[:STATe]**

<b>Command</b>	SYSTem:ULANguage (Query only)
<b>Description</b>	This command queries the language that the instrument uses to display the information on the screen. This command is query only.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:ULANguage?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	ENGLish
<b>Example</b>	SYSTem:ULANguage? Example return: ENGLish, which means that the instrument displays information in English.

**Table 174: SYSTem:ULANguage?**

<b>Command</b>	SYSTem:VERSiOn (Query only)
<b>Description</b>	This command returns the SCPI conformance version of the instrument. This command is query only.
<b>Group</b>	System
<b>Syntax</b>	SYSTem:VERSiOn?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<SCPI Version>::=YYYY.V Where: YYYY indicates the year. V indicates the version number for that year.
<b>Example</b>	SYSTem:VERSiOn? Example return: 1999.0

**Table 175: SYSTem:VERSiOn?**

<b>Command</b>	TRACe[n][:DATA]
<b>Description</b>	This command transfers the waveform data from the external controller to the arbitrary buffer of the selected channel. It's also possible choose which arbitrary buffer select: arbitrary buffer for carrier, modulation or sweep. The query form of this command returns the binary block data. The maximum allowed length is 16384 samples. It's possible to transfer a larger number of samples but only 16384 will be saved in the buffer and the others will be discarded.

	When you send this command, if the instrument is running it will be stopped.
<b>Group</b>	System
<b>Syntax</b>	TRACe[n][:DATA] [{CARrier   MODulation   SWEep}], <binary_block_data> TRACe[n][:DATA]? [{CARrier   MODulation   SWEep}] Where [{CARrier   MODulation   SWEep}] is an optional parameter
<b>Related Commands</b>	None
<b>Arguments</b>	<p>The value of n indicates the channel number.</p> <p>CARrier   MODulation   SWEep specifies the arbitrary buffer target.</p> <p>&lt;binary_block_data&gt; is the waveform data in binary format.</p> <p>Example: #42000&lt;DAB&gt;&lt;DAB&gt;...&lt;DAB&gt;</p> <p>The block data is composed by 4 field:</p> <ul style="list-style-type: none"> <li>• The character “#” that starts the binary block.</li> <li>• The first number (4) indicates number of digits of the byte count field.</li> <li>• The byte count field (2000) tells the length in byte of the transferred data.</li> <li>• &lt;DAB&gt; fields contain the data, each &lt;DAB&gt; is a sample, it is composed by 2 byte that represent an unsigned number between 0 and 65535 in big endian format.</li> </ul> <p>After the reception, the waveform is normalized to output the amplitude and the offset set through the specific commands, then it isn't important the absolute value of the samples, the best choice is to use the full available range, from 0 to 65535.</p>
<b>Returns</b>	<binary_block_data>
<b>Example</b>	TRACe1:DATA CAR,#42000<DAB><DAB>...<DAB> Transmit a waveform of 1000 samples to the carrier arbitrary buffer memory of the channel 1 of the arbitrary function generator.

**Table 176: TRACe[n][:DATA]**

<b>Command</b>	TRACe[n]:POINTs? (Query only)
<b>Description</b>	This command queries the number of data points for the waveform in the arbitrary buffer memory for the specified channel. It's also

	possible choose which arbitrary buffer select: arbitrary buffer for carrier, modulation or sweep. This command is query only.
<b>Group</b>	Trace
<b>Syntax</b>	TRACe[n]:POINTs? [MIN   MAX],[{CARier   MODulation   SWEep}]
<b>Related Commands</b>	None
<b>Arguments</b>	The value of n indicates the channel number. MINimum queries the minimum number of samples. MAXimum queries the maximum number of samples. CARrier   MODulation   SWEep specifies the arbitrary buffer target.
<b>Returns</b>	<NR1>::= number of samples.
<b>Example</b>	TRACe1:POINTs? MAX,CARier Example return: 16384, which is the maximum number of points for arbitrary carrier buffer of channel 1.

**Table 177: TRACe[n]:POINTs?**

<b>Command</b>	TRACe[n]:RECall
<b>Description</b>	This command recalls the contents of arbitrary buffer memory target (carrier, modulation or sweep) for the specified channel from a specified file in the file system. This command works only with ".txt", ".csv" and ".trc" files. There is no query form of this command.
<b>Group</b>	Trace
<b>Syntax</b>	TRACe[n]:RECall <filename>,[{CARier   MODulation   SWEep}]
<b>Related Commands</b>	TRACe[n]:SAVE
<b>Arguments</b>	The value of n indicates the channel number. <filename>::= <Qstring> The file name you want to recall data from. The path can be absolute or relative, if you insert a relative path it starts from Current Working Directory. CARrier   MODulation   SWEep specifies the arbitrary buffer target.
<b>Returns</b>	None
<b>Example</b>	TRACe1:RECall "waveform1.txt",MODulation Recalls the waveform data in the arbitrary modulation buffer of the channel 1 from the file "waveform1.txt". The file is located in the Current Working Directory.

**Table 178: TRACe[n]:RECall**

<b>Command</b>	TRACe[n]:SAVE
<b>Description</b>	This command saves the contents of arbitrary buffer memory target (carrier, modulation or sweep) of the selected channel to a specified

	file in the file system. This command works only with ".txt" file, if the destination file exist and it isn't locked it will be overwritten. There is no query form of this command.
<b>Group</b>	Trace
<b>Syntax</b>	TRACe[n]:SAVE <filename>,{[CARier   MODulation   SWEep]}
<b>Related Commands</b>	TRACe[n]:RECall
<b>Arguments</b>	The value of n indicates the channel number. <filename>::= <Qstring> The name of the file you want to save. The path can be absolute or relative, if you insert a relative path it starts from Current Working Directory. CARier   MODulation   SWEep specifies the arbitrary buffer target.
<b>Returns</b>	None
<b>Example</b>	TRACE1:SAVE "waveform1.txt",SWEep Copies the waveform data in the arbitrary sweep buffer of the channel 1 to the file "waveform1.txt".

**Table 179: TRACe[n]:SAVE**

<b>Command</b>	STATus:OPERation[:EVENT]?
<b>Description</b>	This command returns the value in the Operation Event Register (OEVR) and clears the OEVR. This command is query only.
<b>Group</b>	Status
<b>Syntax</b>	STATus:OPERation[:EVENT]?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<NR1>::=<bit_value>
<b>Example</b>	STATus:OPERation:EVENT? Example return: 2, which indicates that the OEVR contains the binary number 00000010 and the instrument CH2 is waiting for a trigger.

**Table 180: STATus:OPERation[:EVENT]?**

<b>Command</b>	STATus:OPERation:CONDition?
<b>Description</b>	This command returns the contents of the Operation Condition Register (OCR). This command is query only.
<b>Group</b>	Status
<b>Syntax</b>	STATus:OPERation:CONDition?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<NR1>::=<bit_value>



<b>Example</b>	STATus:OPERation:CONDition? Example return: 2, which indicates that the OCR contains the binary number 00000010 and the instrument CH2 is waiting for a trigger.
----------------	---

**Table 181: STATus:OPERation:CONDition?**

<b>Command</b>	STATus:OPERation:ENABLE
<b>Description</b>	This command queries the mask of the Operation Enable Register (OENR). Note that the OENR is not used.
<b>Group</b>	Status
<b>Syntax</b>	STATus:OPERation:ENABLE?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	0
<b>Example</b>	STATus:OPERation:ENABLE?

**Table 182: STATus:OPERation:ENABLE**

<b>Command</b>	STATus:QUESTionable[:EVENT]?
<b>Description</b>	This command returns the value in the Questionable Event Register (QEVr) and clears the QEVr. This command is query only. Note that the QEVr is not used.
<b>Group</b>	Status
<b>Syntax</b>	STATus:QUESTionable[:EVENT]?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	0
<b>Example</b>	STATus:QUESTionable:EVENT?

**Table 183: STATus:QUESTionable[:EVENT]?**

<b>Command</b>	STATus:QUESTionable:CONDition?
<b>Description</b>	This command returns the contents of the Questionable Condition Register (QCR). This command is query only. Note that the QCR is not used.
<b>Group</b>	Status
<b>Syntax</b>	STATus:QUESTionable:CONDition?
<b>Related Commands</b>	
<b>Arguments</b>	None

<b>Returns</b>	0
<b>Example</b>	STATus:QUESTIONable:CONDition?

**Table 184: STATus:QUESTIONable:CONDition?**

<b>Command</b>	STATus:QUESTIONable:ENABLE
<b>Description</b>	This command queries the mask for the Questionable Enable Register (QENR). Note that the QENR is not used.
<b>Group</b>	Status
<b>Syntax</b>	STATus:QUESTIONable:ENABLE?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	0
<b>Example</b>	STATus:QUESTIONable:ENABLE?

**Table 185: STATus:QUESTIONable:ENABLE**

<b>Command</b>	STATus:PRESet
<b>Description</b>	This command presets the SCPI status registers (Operation Enable Register (OENR) and Questionable Enable Register (QENR)). There is no query form of this command.
<b>Group</b>	Status
<b>Syntax</b>	STATus:PRESet
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	STATus:PRESet Presets the SCPI status registers.

**Table 186: STATus:PRESet**

<b>Command</b>	*CLS
<b>Description</b>	This command clears all the event registers in Standard Event Status Register (SESR), the Status Byte Register SBR (except the MAV bit) and queues that are used in the arbitrary function generator status and event reporting system. There is no query form of this command
<b>Group</b>	Status
<b>Syntax</b>	*CLS
<b>Related Commands</b>	None
<b>Arguments</b>	None

<b>Returns</b>	None
<b>Example</b>	*CLS Clear all the event registers and queues.

**Table 187: \*CLS**

<b>Command</b>	*ESE
<b>Description</b>	This command sets or queries the bits in the Event Status Enable Register (ESER) used in the status and events reporting system of the arbitrary function generator. The ESER prevents events from being reported to the Status Byte Register (STB). The query form of this command returns the contents of the ESER.
<b>Group</b>	Status
<b>Syntax</b>	*ESE <bit_value> *ESE?
<b>Related Commands</b>	*CLS *ESR? *SRE *STB?
<b>Arguments</b>	<NR1>::=<bit_value>
<b>Returns</b>	<bit_value>
<b>Example</b>	*ESE 177 Sets the ESER to 177 (binary 10110001), which determines that the PON, CME, EXE, and OPC bits should be set in SBR register. *ESE? Example return: 186, which indicates that the ESER contains the binary value 10111010.

**Table 188: \*ESE**

<b>Command</b>	*ESR?
<b>Description</b>	This command returns the contents of the Standard Event Status Register (SESR) used in the status events reporting system in the arbitrary function generator. This command clears the SESR when it reads it. This command is query only.
<b>Group</b>	Status
<b>Syntax</b>	*ESR?
<b>Related Commands</b>	*CLS *ESE? *SRE

	*STB?
<b>Arguments</b>	None
<b>Returns</b>	<NR1> Indicates that the contents of the SESR is a decimal integer.
<b>Example</b>	*ESR? Example return: 181, which indicates that the SESR contains the binary number 10110101.

**Table 189: \*ESR?**

<b>Command</b>	*SRE
<b>Description</b>	This command sets and queries the bits in the Service Request Enable Register (SRER).
<b>Group</b>	Status
<b>Syntax</b>	*SRE <bit_value> *SRE?
<b>Related Commands</b>	None
<b>Arguments</b>	<bit_value>::=<NR1> Where: <NR1> is a value from 0 through 255. The binary bits of the SRER are set according to this value. Using an out-of-range value causes an execution error.
<b>Returns</b>	<bit_value>
<b>Example</b>	*SRE 48 Set the bits in the SRER to binary 00110000. *SRE? Example return: 32, which means that the bits in the SRER have the binary value of 00100000

**Table 190: \*SRE**

<b>Command</b>	*STB?
<b>Description</b>	This command returns the contents of the Status Byte Register (SBR) using the Master Summary Status (MSS) bit. This command is query only.
<b>Group</b>	Status
<b>Syntax</b>	*STB?
<b>Related Commands</b>	None
<b>Arguments</b>	<bit_value>::=<NR1> Where: <NR1> is a value from 0 through 255. The binary bits of the SRER are set according to this value. Using an out-of-range value causes an execution error.

<b>Returns</b>	<NR1>
<b>Example</b>	*STB? Example return: 96, which indicates that the SBR contains the binary value 01100000.

**Table 191: \*STB?**

<b>Command</b>	*OPC
<b>Description</b>	This command generates the operation complete message by setting bit 0 in the Standard Event Status Register (SESR) when all pending commands that generate an OPC message are complete. The query version of this command places the ASCII character "1" into the output queue when all such *OPC commands are complete.
<b>Group</b>	Synchronization
<b>Syntax</b>	*OPC *OPC?
<b>Related Commands</b>	None
<b>Arguments</b>	None
<b>Returns</b>	<execution complete>::=1 Where: "1" indicates that all pending operations are complete.
<b>Example</b>	*OPC? Example return if all pending OPC operations are finished: 1. The arbitrary function generator always returns 1.

**Table 192: \*OPC**

<b>Command</b>	*WAI
<b>Description</b>	This command prevents the instrument from executing further commands or queries until all pending commands that generate an operation complete (OPC) message are complete. There is no query form of this command.
<b>Group</b>	Synchronization
<b>Syntax</b>	*WAI
<b>Related Commands</b>	*OPC
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	*WAI Prevent the instrument from executing any further commands or queries until all pending commands that generate an OPC message are complete.

**Table 193: \*WAI**

<b>Command</b>	*TRG
<b>Description</b>	This command generates a trigger event. There is no query form of this command.
<b>Group</b>	Trigger
<b>Syntax</b>	*TRG
<b>Related Commands</b>	ABORT TRIGger[:SEquence][:IMMediate]
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	*TRG Generate a trigger event.

**Table 194: \*TRG**

<b>Command</b>	TRIGger[:SEquence][:IMMediate]
<b>Description</b>	This command forces a trigger event to occur. There is no query form of this command.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEquence][:IMMediate]
<b>Related Commands</b>	ABORT *TRG
<b>Arguments</b>	None
<b>Returns</b>	None
<b>Example</b>	TRIGger:SEquence:IMMediate Generate a trigger event.

**Table 195: TRIGger[:SEquence][:IMMediate]**

<b>Command</b>	ABORT
<b>Description</b>	This command resets the trigger event. There is no query form of this command.
<b>Group</b>	Trigger
<b>Syntax</b>	ABORT
<b>Related Commands</b>	*TRG TRIGger[:SEquence][:IMMediate]
<b>Arguments</b>	None
<b>Returns</b>	None

<b>Example</b>	ABORT Reset the trigger system
----------------	-----------------------------------

**Table 196: ABORT**

<b>Command</b>	TRIGger[:SEQuence]:SOURce
<b>Description</b>	This command sets or queries the instrument trigger source.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEQuence]:SOURce {TIMER   EXTERNAL   MANUAL} TRIGger[:SEQuence]:SOURce?
<b>Related Commands</b>	None
<b>Arguments</b>	<source>::= {TIMER   EXTERNAL   MANUAL} TIMER: the trigger is sent at regular intervals. EXTERNAL: the trigger come from the external BNC connector. MANUAL: the trigger is sent via software or using the trigger button on front panel.
<b>Returns</b>	TIM   EXT   MAN
<b>Example</b>	TRIGger:SOURce TIMER It sets the trigger source to timer. TRIGger:SOURce? Might return TIMER

**Table 197: TRIGger[:SEQuence]:SOURce**

<b>Command</b>	TRIGger[:SEQuence]:SLOPe
<b>Description</b>	This command sets or queries the instrument trigger input slope for the external source.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEQuence]: SLOPe {RISING   FALLING   BOTH} TRIGger[:SEQuence]: SLOPe?
<b>Related Commands</b>	TRIGger[:SEQuence]:SOURce
<b>Arguments</b>	<slope>::= {RISING   FALLING   BOTH}
<b>Returns</b>	<slope>
<b>Example</b>	TRIGger:SLOPe RISING It sets the trigger slope to rising edge. TRIGger:SLOPe? Might return RISING.

**Table 198: TRIGger[:SEQuence]:SLOPe**

<b>Command</b>	TRIGger[:SEQuence]:THREshold
<b>Description</b>	This command sets or queries the threshold of an external trigger signal when you select the external trigger input as trigger source with the TRIGger[:SEQuence]:SOURce command.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEQuence]:THREshold <threshold> TRIGger[:SEQuence]:THREshold? [MINimum   MAXimum]
<b>Related Commands</b>	TRIGger[:SEQuence]:SOURce
<b>Arguments</b>	<threshold>::= <NRf>[<units>] Where: <units>::=[mV   V] MINimum queries the minimum threshold level. MAXimum queries the maximum threshold level.
<b>Returns</b>	<threshold>
<b>Example</b>	TRIGger:SEQuence:THREshold 1 Set the external trigger input level to 1 V.

**Table 199: TRIGger[:SEQuence]:THREshold**

<b>Command</b>	TRIGger[:SEQuence]:TIMer
<b>Description</b>	This command sets or queries the timer for the trigger event.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEQuence]:TIMer <interval> TRIGger[:SEQuence]:TIMer? [MINimum   MAXimum]
<b>Related Commands</b>	TRIGger[:SEQuence]:SOURce
<b>Arguments</b>	<interval>::=<NRf> [<units>] Where: <NRf> is the timer value <units>::=[us   ms   s] MINimum queries the minimum time interval. MAXimum queries the maximum timer interval.
<b>Returns</b>	<interval>
<b>Example</b>	TRIGger:TIMer 0.5 It sets the trigger timer to 0.5 seconds. TRIGger:TIMer? MAXimum It might return 100 seconds

**Table 200: TRIGger[:SEQuence]:TIMer**

<b>Command</b>	TRIGger[:SEQuence]:IMPedance
----------------	------------------------------



<b>Description</b>	This command sets or queries the impedance of an external trigger signal when you select the external trigger input as trigger source with the TRIGger[:SEQuence]:SOURce command.  It can be 50 Ohm or 1 KOhm
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[:SEQuence]: IMPedance {50Ohm,1KOhm} TRIGger[:SEQuence]: IMPedance?
<b>Related Commands</b>	TRIGger[:SEQuence]:SOURce
<b>Arguments</b>	<impedance>::= {50Ohm   1KOhm} Where: 50Ohm is 50 Ohm selection. 1KOhm is 1K Ohm selection.
<b>Returns</b>	< impedance>
<b>Example</b>	TRIGger:IMPedance 50Ohm It sets the trigger impedance to 50Ohm. TRIGger:IMPedance? It might return 50Ohm

**Table 154: TRIGger[:SEQuence]:IMPedance**

<b>Command</b>	TRIGger[m]:OUTPut:AMPLitude
<b>Description</b>	This command sets or queries the marker out voltage level for the specified channel.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[m]:OUTPut:AMPLitude <voltage level> TRIGger[m]:OUTPut:AMPLitude? {MINimum   MAXimum}
<b>Related Commands</b>	None
<b>Arguments</b>	Where m indicates the marker out channel. <level>::=<NRf>[<units>] Where: <NRf> is the trigger output high level. <units>::=[V   mV]. MINimum queries the minimum level. MAXimum queries the maximum level.
<b>Returns</b>	<voltage level>
<b>Example</b>	TRIGger1:OUTPut:AMPLitude 2 It sets the marker out voltage to 2 Volts. TRIGger1:OUTPut:AMPLitude? MIN It might return 1 Volts.

**Table 201: TRIGger[m]:OUTPut:AMPLitude**

<b>Command</b>	TRIGger[m]:OUTPut:DElay
<b>Description</b>	This command sets or queries the marker out delay.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[1   2   3   4]:OUTPut:DElay <skew> TRIGger[1   2   3   4]:OUTPut:DElay? [MINimum   MAXimum]
<b>Related Commands</b>	None
<b>Arguments</b>	Where m indicates the marker out channel. <skew>:=<NRf> [<units>] Where: <NRf> is the timer value <units>::=[ns   us   ms   s]
<b>Returns</b>	<skew>
<b>Example</b>	TRIGger1:OUTPut:DElay 1ns It sets the marker out delay to 1 ns. TRIGger1:OUTPut:DElay? MAXimum It might return 100 nanoseconds.

**Table 202: TRIGger[m]:OUTPut:DElay**

<b>Command</b>	TRIGger[m]:OUTPut[:STATE]
<b>Description</b>	This command sets or queries the marker output state and enable or disable the the marker out.
<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[m]:OUTPut:STATe {ON   OFF   0   1} TRIGger[m]:OUTPut:STATe?
<b>Related Commands</b>	None
<b>Arguments</b>	Where m indicates the marker out channel. ON   1 enables the marker out for the specified channel. OFF   0 disables the marker out for the specified channel.
<b>Returns</b>	<NR1> 0 means OFF, 1 means ON
<b>Example</b>	TRIGger1:OUTPut:STATe ON Enable the marker out for the channel 1.

**Table 203: TRIGger[m]:OUTPut:STATe**

<b>Command</b>	TRIGger[m]:OUTPut:LINK <output>
<b>Description</b>	This command sets or queries links the marker output to the selected output.  <i>Important Note:</i> On Model 675 series each marker out can be assigned to the couple of outputs [1   2],[3   4],[5   6],[7   8]

<b>Group</b>	Trigger
<b>Syntax</b>	TRIGger[m]:OUTPut:LINK <output> TRIGger[m]:OUTPut:LINK?
<b>Related Commands</b>	None
<b>Arguments</b>	Where m indicates the marker out channel. <output>:=<NR1> Where: <NR1> is a value from 1 through 8 that means the output channel number assigned to the marker out.
<b>Returns</b>	<output channel>
<b>Example</b>	TRIGger1:OUTPut:LINK 2 Links the marker output channel 1 to the channel 2. TRIGger1:OUTPut:LINK? It might return 2

Table 204 TRIGger[m]:OUTPut:LINK

## 5. COMMAND ERRORS

Command errors are returned when there is a syntax error in the command.

Error code	Error message
-369	Out of Range Channel Coupling Error: the formula result is out of range
-368	Channel Coupling Error: it is not possible to couple this parameter
-365	Time Out Error
-360	Communication Error
-350	Queue Overflow
-340	Calibration Error
-330	Self Test Failed
-321	Out of Memory
-320	Storage Fault
-316	Instrument Setting Error
-314	Save/Recall Memory Lost
-313	Calibration Memory Lost
-311	Memory Error
-310	System Error
-307	License Error

-306	Waveform Range Error
-305	Waveform Length Error
-303	Waveform Not Found
-302	Error to parsing waveform block data
-301	Channels Error
-300	Device Specific Error
-250	File Error
-223	Parameter disabled and not modifiable
-222	Out of Range Error
-221	Invalid run mode: the AFG is not in the correct run mode for this operation
-104	Data Type Error
0	No error
5	Too many numeric suffices in Command Spec
10	No Input Command to parse
14	Numeric suffix is invalid value
16	Invalid value in numeric or channel list (the value doesn't meet the parameters already set)
17	Invalid number of dimensions in a channel list
20	Parameter of type Numeric Value overflowed its storage
30	Wrong units for parameter
40	Wrong type of parameter(s)
50	Wrong number of parameters
60	Unmatched quotation mark (single/double) in parameters
65	Unmatched bracket
70	Command keywords were not recognized
200	No entry in list to retrieve (number list or channel list)
210	Too many dimensions in entry to be returned in parameters
220	; plus End of line commands

## 6. PROGRAMMING EXAMPLES

The AFG-SDK contains several example scripts and other examples written using LabView, Microsoft Visual C++, Microsoft C# .NET, Python, Matlab.

The programs run on Microsoft Windows® PC-compatible systems equipped with NIVISA.

NI-VISA is the National Instruments implementation of the VISA I/O standard. NI-VISA includes software libraries, interactive utilities such as NI I/O Trace and the VISA Interactive Control, and configuration programs through Measurement & Automation Explorer for all your development needs.

Use NIVISA in software to write interoperable instrument drivers to handle communicating between software applications and your instrument.

You can download the latest version of NIVISA tools here:

<http://search.ni.com/nisearch/app/main/p/bot/no/ap/tech/lang/it/pg/1/sn/catnav:du,n8:3.1637.ssnv:sup/>

The example programs assume that the system recognizes the PC (external controller) resource name.

Refer to the NIVISA section of this manual for details about resource names.

### 6.1 Example Script

In the folder you can find some text files that show the use of the SCPI commands that controls the main features of the Function Generator. You can send them to the instrument using the AT-Instrument-Communicator.

### 6.2 Python examples

The Python examples are developed using Python 3.7 32 bit, they show how to communicate with the instrument and how to send a waveform to the instrument memory and generate the signal.

The communication is based on NI VISA, then before run these examples it is necessary to download and install the “pyvisa” that is the VISA version for Python language.


### 6.3 Matlab examples

The Matlab examples are developed using Matlab R2014b, in the folder you can find 2 files:

- Send\_Wfm\_Binary\_Block: this function sends the samples from Matlab workspace to the instrument memory;
- Generation\_Example: this example creates a parabolic waveform and send it to the instrument using the function showed above. When the generation started on channel 1 there is the parabolic waveform and on the channel 2 there is Sinc function from the instrument predefined. You can change some parameter such as Amplitude, Offset, Frequency and for the function generated in Matlab workspace you can change the Number of Samples and the function.


### 6.4 LabView examples

The LabView examples require at least LabView 2013 64 bit version, you should copy SDK\_AFG SDK\_AFG\_4010\_Rev\Active Technologies AFG3000 folder in ...\\LabVIEW 2013\\instr.lib folder on your computer and open the file Active Technologies AFG3000.lvproj.

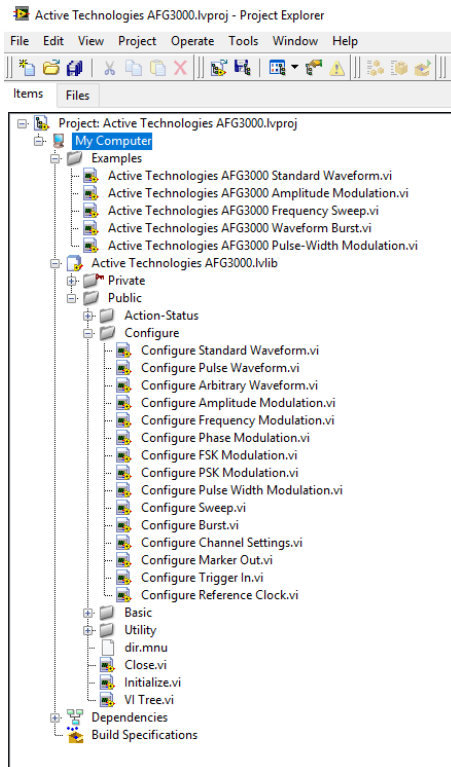

The LabView project contains several Vis that control the basic instrument features and five examples located in the folder *Examples*.

Double click on the project tree to launch the *Active\_Technologies\_AFG3000\_Standard\_Waveform.vi* example

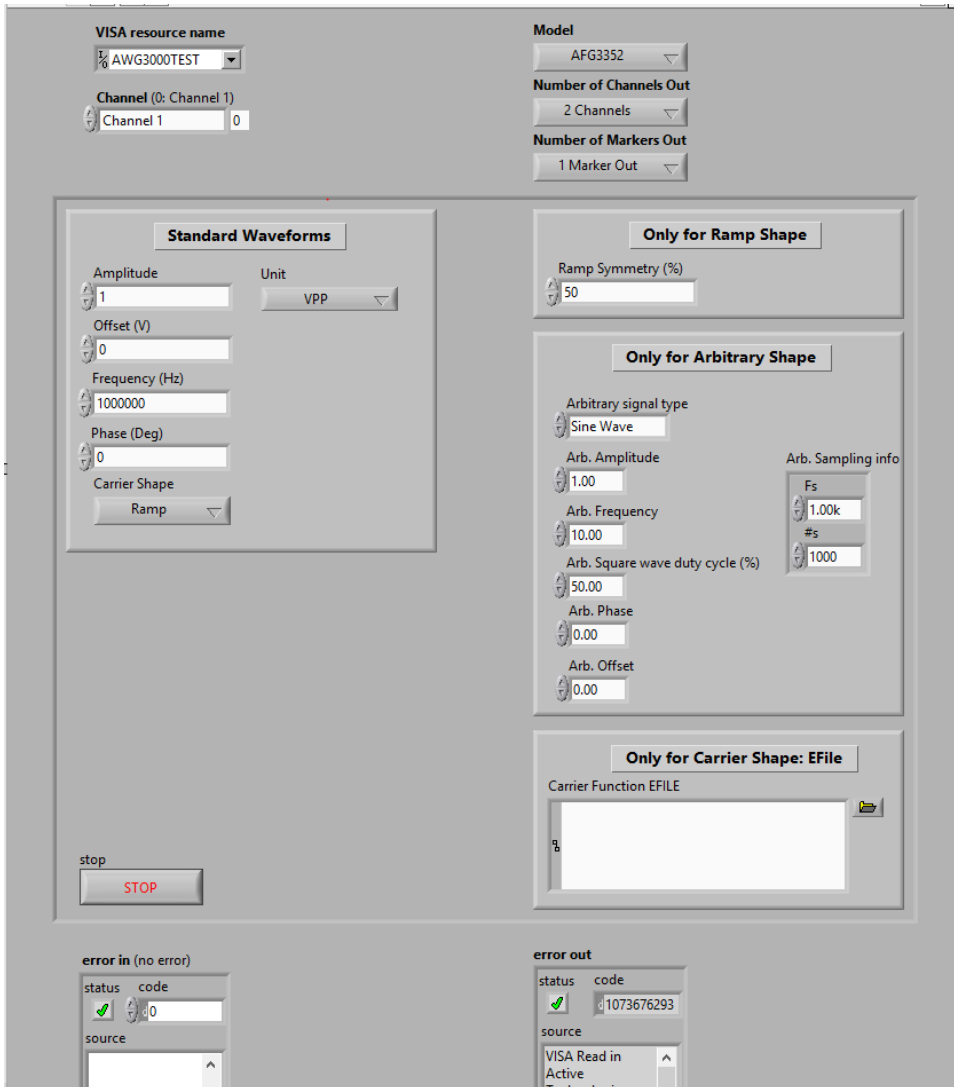


This example generates a standard waveform (Sine, Square, Ramp, Pulse, Sync, Gaussian, Lorentz, Exponential, Haversine) in Continuous Mode; before running the VI, you should select the AFG 3000 resources in the VISA resource name control.

You can change the Amplitude, Frequency, Offset, Phase and Symmetry (only for Ramp waveform) output parameters on the fly while the instrument is running.

You can generate an arbitrary waveform selecting from a file (Efile) or an array of sample (connect to the *Basic Function Generator VI* in this example). A Pseudo Random Noise and a DC Level could also be generated.

Run the VI to start the generation, press the STOP button to stop the waveform generation.

Double click on the project tree to open the *Active\_Technologies\_AFG3000\_Waveform\_Burst.vi* example

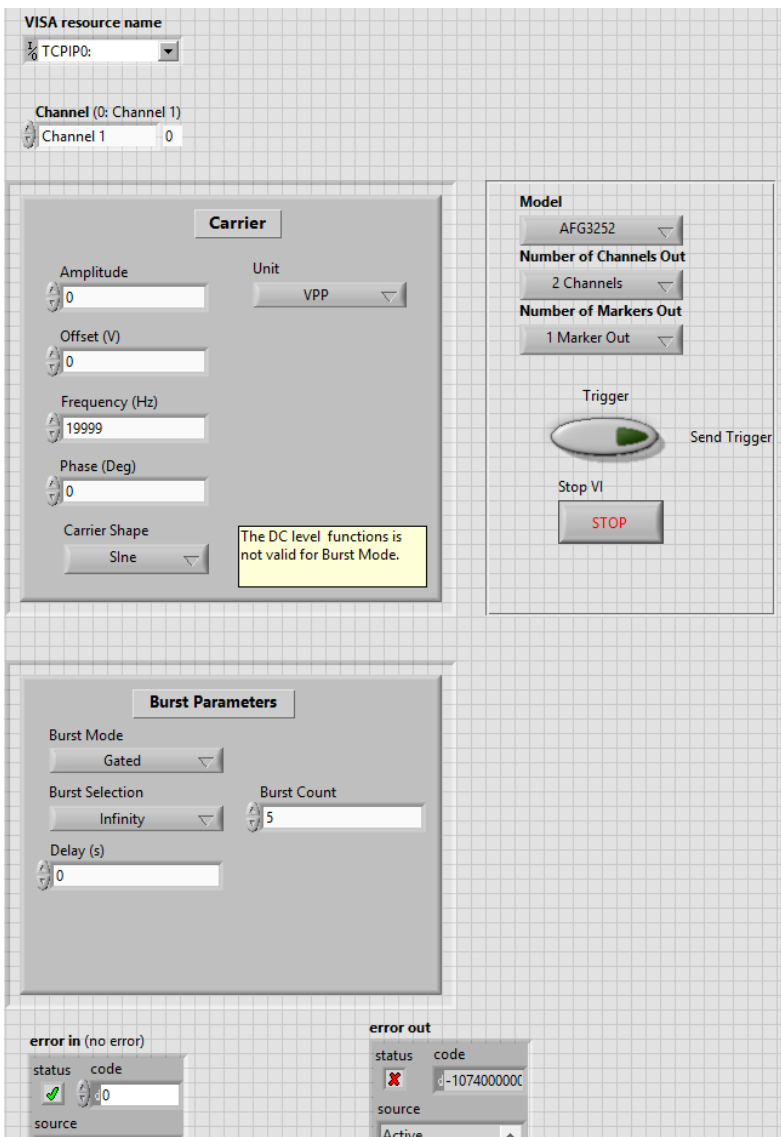




This example generates waveforms in Burst mode for the selected Channel; you can choose the carrier shape (DC waveform is not valid in this mode) and change Amplitude, Frequency, Offset and Phase parameters.

You can also select between Trigger and Gated Mode (consult Model 675\_UserManual for more informations about these two modality).

Run the VI to initialize the instrument and load the default parameters into the instrument; the Send Trigger button starts the waveform burst.

Press the STOP button to stop the waveform generation.

Double click on the project tree to open the Active\_Technologies\_AFG3000\_Frequency\_Sweep.vi example

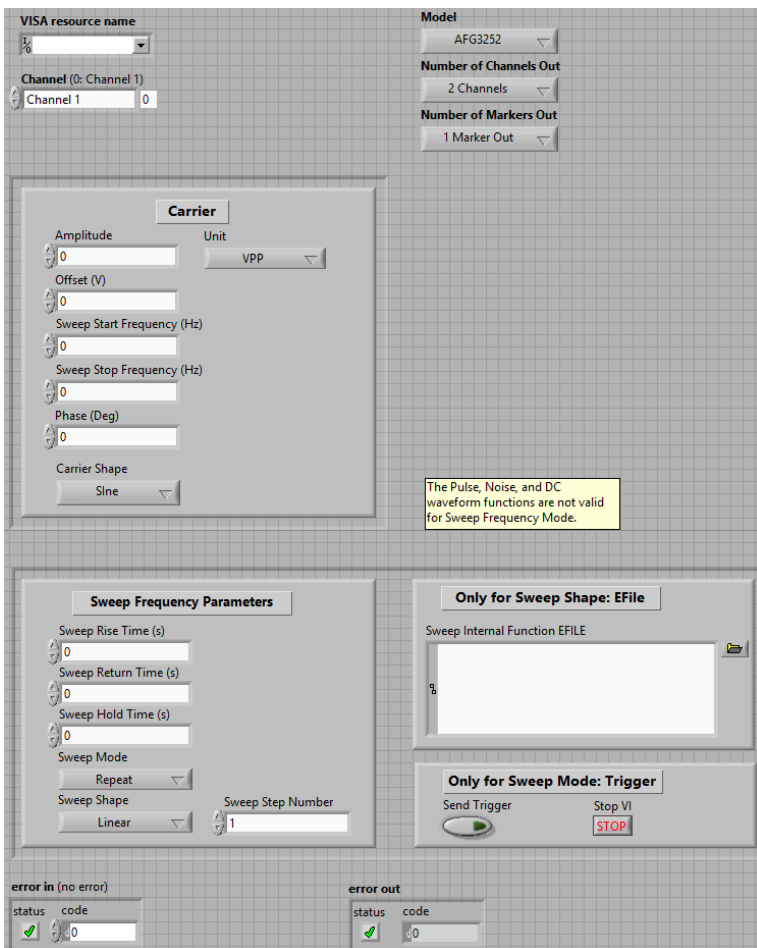


This VI generates a frequency sweep of a carrier waveform (note that Pulse, PR Noise and DC are not valid waveforms in sweep mode). The sweep parameters that you can change are Amplitude, Offset, Phase, Start Frequency(Hz), Stop Frequency(Hz), Return Time(s), Rise Time(s) and Hold Time(s).

You can also choose the profile of the Frequency Sweep (Sweep Shape option).

Run the VI to initialize the instrument parameters and start the generation; only for Trigger Sweep Mode press the SEND TRIGGER button to start the frequency sweep, press the STOP button to stop the waveform generation.


Double click on the project tree to open the Active\_Technologies\_AFG3000\_Amplitude\_Modulation.vi example

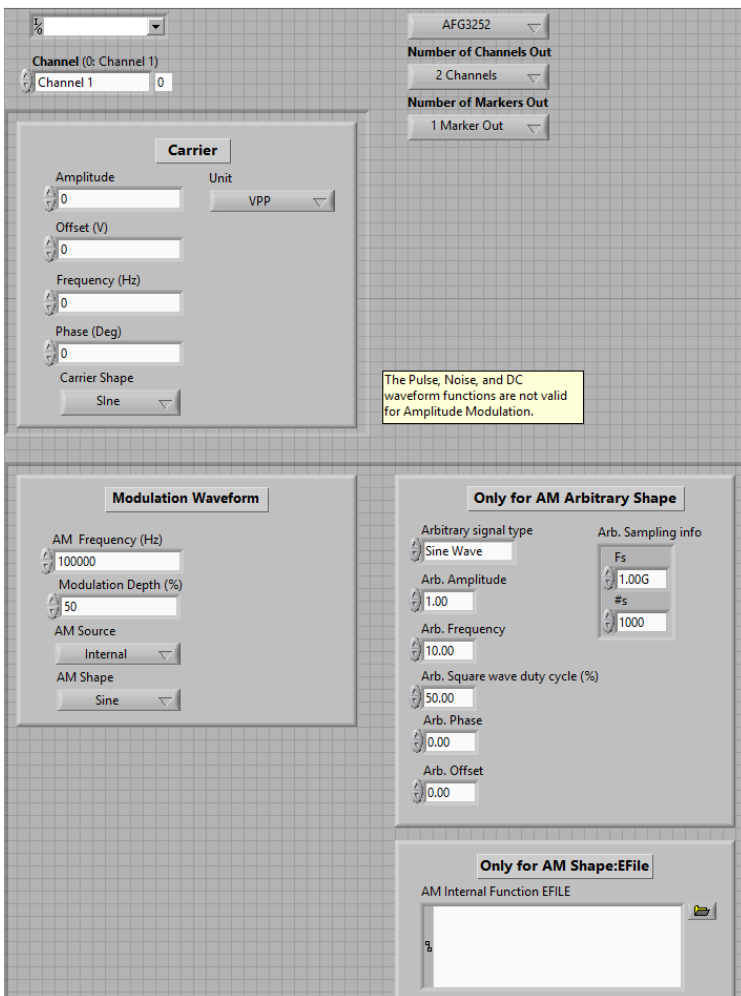

This VI generates an amplitude modulated waveform starting from a carrier defined by Shape, Amplitude, Frequency, Offset and Phase parameters (Pulse, PR Noise and DC are not valid waveforms in AM mode).

You can change the AM frequency, the modulation Depth, the AM source (internal waveform or external from a SMA connector) and Shape.

Double click on the project tree to open the Active\_Technologies\_AFG3000\_Pulse-Width\_Modulation.vi example

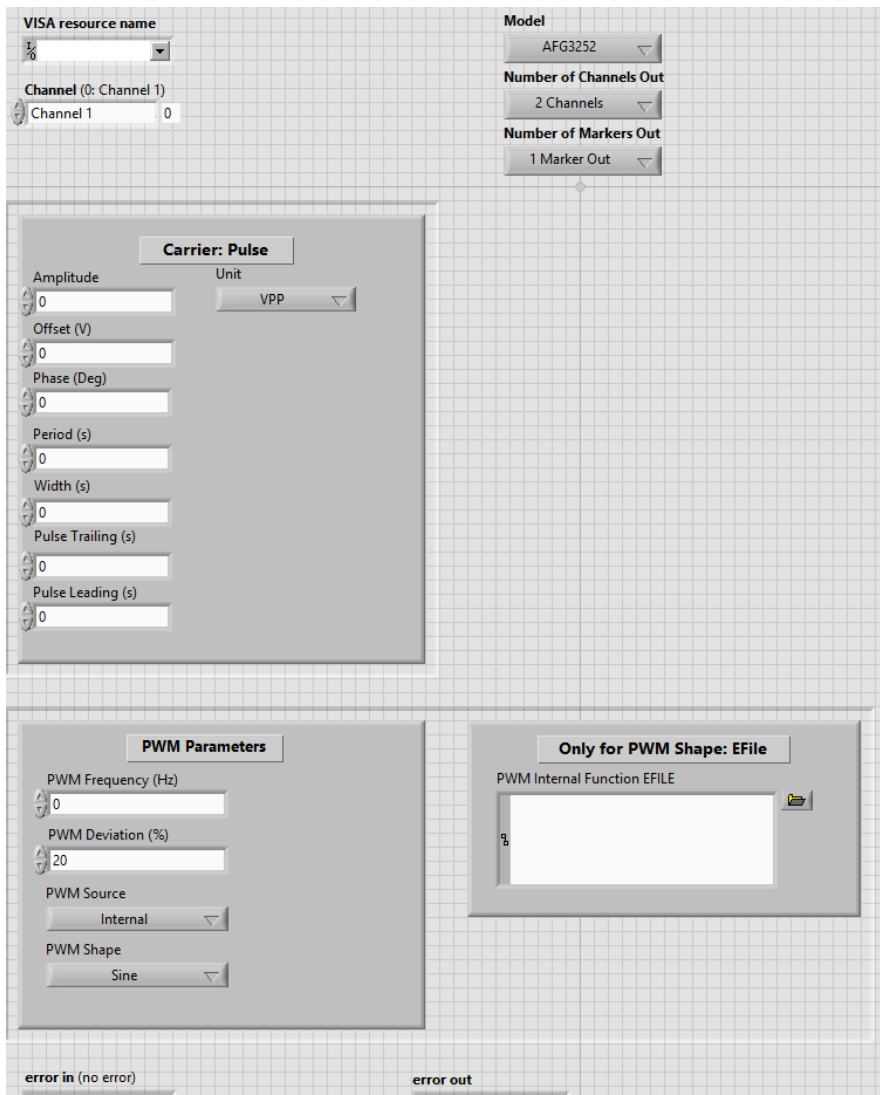


The PWM modulation is the only modulation supported by the Pulse waveform, so the carrier waveform is set Pulse by default.


You can change the rectangular Width, Period, duration of Trailing edge, duration of Leading edge and Deviation of the PWM every time you launch the vi (note that all of the previous parameters are linked each others and the deviation has to meet some particular conditions, consult the Model 675\_UserManual for more details).

## 6.5 Microsoft C# Example

The C# example is located under the folder AT\_AFG\_Rider\_3000\_Series\_VS2017\_Examples, you need to install Microsoft Visual Studio 2017 to open and launch the solution.

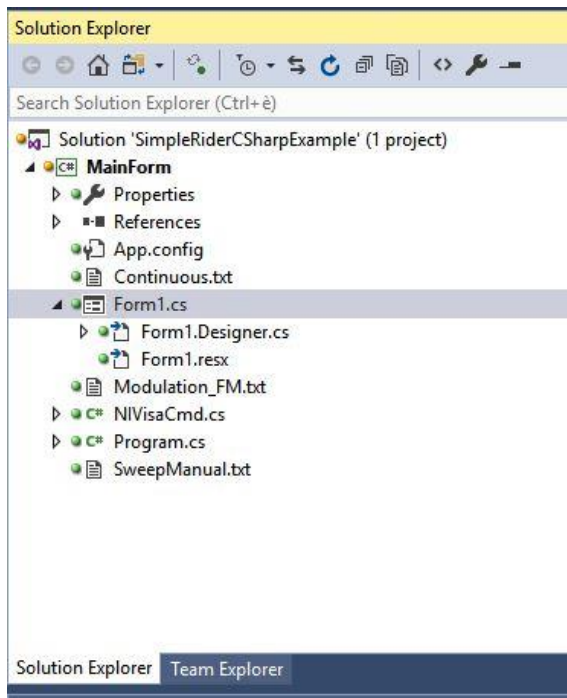

You should compile and launch the example; in the form you have to write the Instrument Address and press the Connect button to establish a connection with the instrument. If the connection works correctly, the instrument should respond to the \*IDN? command in the Server Answer textbox.

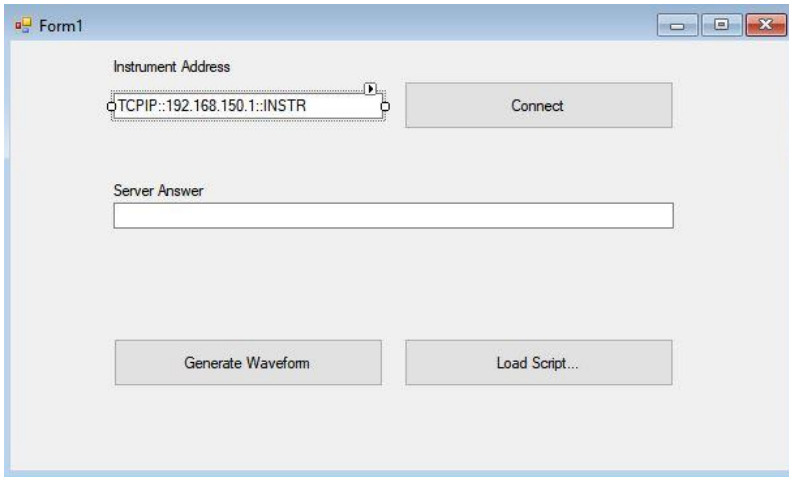

Clicking on the Generate Waveform button, you will send several SCPI commands to the instrument that will generate a single pulse waveform in Continuous mode.

```
private void btnGenerateWave_Click(object sender, EventArgs e)
{
    // Reset to default
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "*RST");
    // Set the channel 1 parameters
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "SOURce1:FUNCTION:SHAPE SINusoid");
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "SOURce1:FREQuency 100MHZ");
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "SOURce1:VOLTage:AMPLitude 1");
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "SOURce1:VOLTage:OFFSet 0");
    // Set the channel 2 parameters
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "SOURce2:FUNCTION:SHAPE SQUARE");
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "SOURce2:FREQuency 5MHZ");
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "SOURce2:VOLTage:HIGH 2");
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "SOURce2:VOLTage:LOW 0");
    //Turn on the output channels
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "OUTPut1:STATE ON");
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "OUTPut2:STATE ON");
    //Start the generation
    tbAnswer.Text = vs.SendTo(sInstrumentAddress, "AFGControl:START");
}
}
```

The *Load Script...* button lets you to load a SCPI command script file; in the project folder there are three available scripts *Continuous.txt*, *Modulation\_FM.txt* and *Sweep.txt*.

## 6.6 Microsoft C++ Example

The C++ example is located under the folder AT\_AFG\_Rider\_3000\_Series\_VS2017\_Examples\AFGRiderMSVC\TCPIP

The example is written in Microsoft® Visual C++

```
#include "visa.h"

#include <stdio.h>
#include <stdlib.h>
#include <string>

static char outputBuffer[VI_FIND_BUFLen];
static ViSession defaultRM, instr;
static ViStatus status;
static ViUInt32 count;
static char acBuffer[10000000] = "";
static unsigned int u32Timeout = 20000; //timeout value in milliseconds

static const char acInstrument[] = "TCPIP::192.168.150.1::INSTR"; // instrument address

ViStatus VisaWrite(std::string sInput)
{
    printf("viWrite - %s \n", sInput.c_str());

    status = viWrite (instr, (ViBuf)sInput.c_str(), sInput.length(), &count);

    if (status < VI_SUCCESS)
    {
        viStatusDesc(instr, status, outputBuffer);
        printf("viWrite failed with error code %x - %s\n", status, outputBuffer);
        viClose(defaultRM);
        exit (EXIT_FAILURE);
    }

    // In case of query command, retrieve the output string
    memset(outputBuffer, 0, sizeof(outputBuffer));

    status = viRead (instr, (ViBuf)outputBuffer, sizeof(outputBuffer), &count);

    if (status < VI_SUCCESS)
    {
        viStatusDesc(instr, status, outputBuffer);
        printf("viRead failed with error code %x - %s\n", status, outputBuffer);
        viClose(defaultRM);
        exit (EXIT_FAILURE);
    }

    outputBuffer[strlen(outputBuffer)-1] = 0;

    if(strlen(outputBuffer) > 0)
```

```

    {
        printf("The server response is:\n %s\n\n",outputBuffer);
    }

    return status;
}

int main()
{
    int iIndex = 0;
    FILE* pFile = NULL;
    ViFindList objFindList;

    /* First we will need to open the default resource manager. */
    status = viOpenDefaultRM (&defaultRM);
    if (status < VI_SUCCESS)
    {
        printf("Could not open a session to the VISA Resource Manager!\n");
        exit (EXIT_FAILURE);
    }

    status = viFindRsrc (defaultRM, "?*INSTR", &objFindList, &count, outputBuffer);
    if (status < VI_SUCCESS)
    {
        viStatusDesc(instr, status, outputBuffer);
        printf("viFindRsrc failed with error code %x - %s\n", status, outputBuffer);
        exit (EXIT_FAILURE);
    }

    printf("viFindRsrc - %s\n", outputBuffer);

    /* Now we will open a session via TCP/IP */
    status = viOpen (defaultRM, (ViRsrc) acInstrument, VI_NULL, u32Timeout, &instr);
    if (status < VI_SUCCESS)
    {
        printf ("An error occurred opening the session to %s\n", acInstrument);
        viClose(defaultRM);
        exit (EXIT_FAILURE);
    }

    // Set the timeout attribute
    viSetAttribute (instr, VI_ATTR_TMO_VALUE, u32Timeout);

    //Identify and reset the instrument
    VisaWrite("*:IDN?");
    VisaWrite("*:RST");
    //Set the Channel 1 Parameters
    VisaWrite("SOURce1:FUNCTION PULSe");
    VisaWrite("SOURce1:PULSe:DCYCLe 60");
    VisaWrite("SOURce1:PULSe:DELay 0");
    VisaWrite("SOURce1:PULSe:PERiod 200ns");
    VisaWrite("SOURce1:PULSe:TRANSition:LEADIng 10ns");
}

```

```

VisaWrite("SOURce1:PULSe:TRANSition:TRAIling 20ns");
VisaWrite("SOURce1:VOLTage:HIGH 2");
VisaWrite("SOURce1:VOLTage:LOW 0");
//Set the Channel 2 Parameters
VisaWrite("SOURce2:FUNCTion SINusoid");
VisaWrite("SOURce2:VOLTage 3");
VisaWrite("SOURce2:VOLTage:OFFSet 0");
VisaWrite("SOURce2:FREQuency 10MHz");
VisaWrite("SOURce1:FREQuency:MODE CW");
VisaWrite("SOURce2:FREQuency:MODE CW");
// Turn On the Outputs
VisaWrite("OUTPut1 ON");
VisaWrite("OUTPut2 ON");
// Start the generation
VisaWrite("AFGControl:START");
status = viClose (instr);
status = viClose (defaultRM);
printf ("\nHit enter to continue.");
fflush(stdin);
getchar();

return 0;
}

```